

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062822.D
 Acq On : 14 Sep 2024 21:57
 Operator : JU/RC
 Sample : P3898-07DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC57DL

Quant Time: Sep 15 01:36:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	42678	20.000	ng/u1	0.00
20) Naphthalene-d8	10.695	136	177470	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.531	164	149396	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.275	188	420301	20.000	ng/u1	0.00
79) Chrysene-d12	21.523	240	469838	20.000	ng/u1	0.00
88) Perylene-d12	24.584	264	526698	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	3.779	84	5052	1.681	ng/u1	0.01
7) Phenol-d5	7.075	99	5680	1.518	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	3092	1.378	ng/u1	0.00
11) 2-Chlorophenol-d4	7.434	132	4172	1.530	ng/u1	0.00
15) 4-Methylphenol-d8	8.603	113	4238	1.359	ng/u1	0.00
21) Nitrobenzene-d5	9.055	128	2189	1.726	ng/u1	0.00
24) 2-Nitrophenol-d4	9.784	143	2091	1.507	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.319	165	4813	1.593	ng/u1	0.00
31) 4-Chloroaniline-d4	10.830	131	5825	1.403	ng/u1	0.00
46) Dimethylphthalate-d6	13.932	166	20395	1.773	ng/u1	0.00
49) Acenaphthylene-d8	14.220	160	22694	1.776	ng/u1	0.00
54) 4-Nitrophenol-d4	14.737	143	1677	0.858	ng/u1	0.00
60) Fluorene-d10	15.524	176	19842	1.914	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.375	188	37967	1.914	ng/u1	0.00
81) Pyrene-d10	19.661	212	50957	1.927	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.373	264	51568	1.854	ng/u1	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.154	232	9930	2.934	ng/u1#	96
71) Pentachlorophenol	16.929	266	171402	51.894	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062822.D
Acq On : 14 Sep 2024 21:57
Operator : JU/RC
Sample : P3898-07DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC57DL

Quant Time: Sep 15 01:36:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

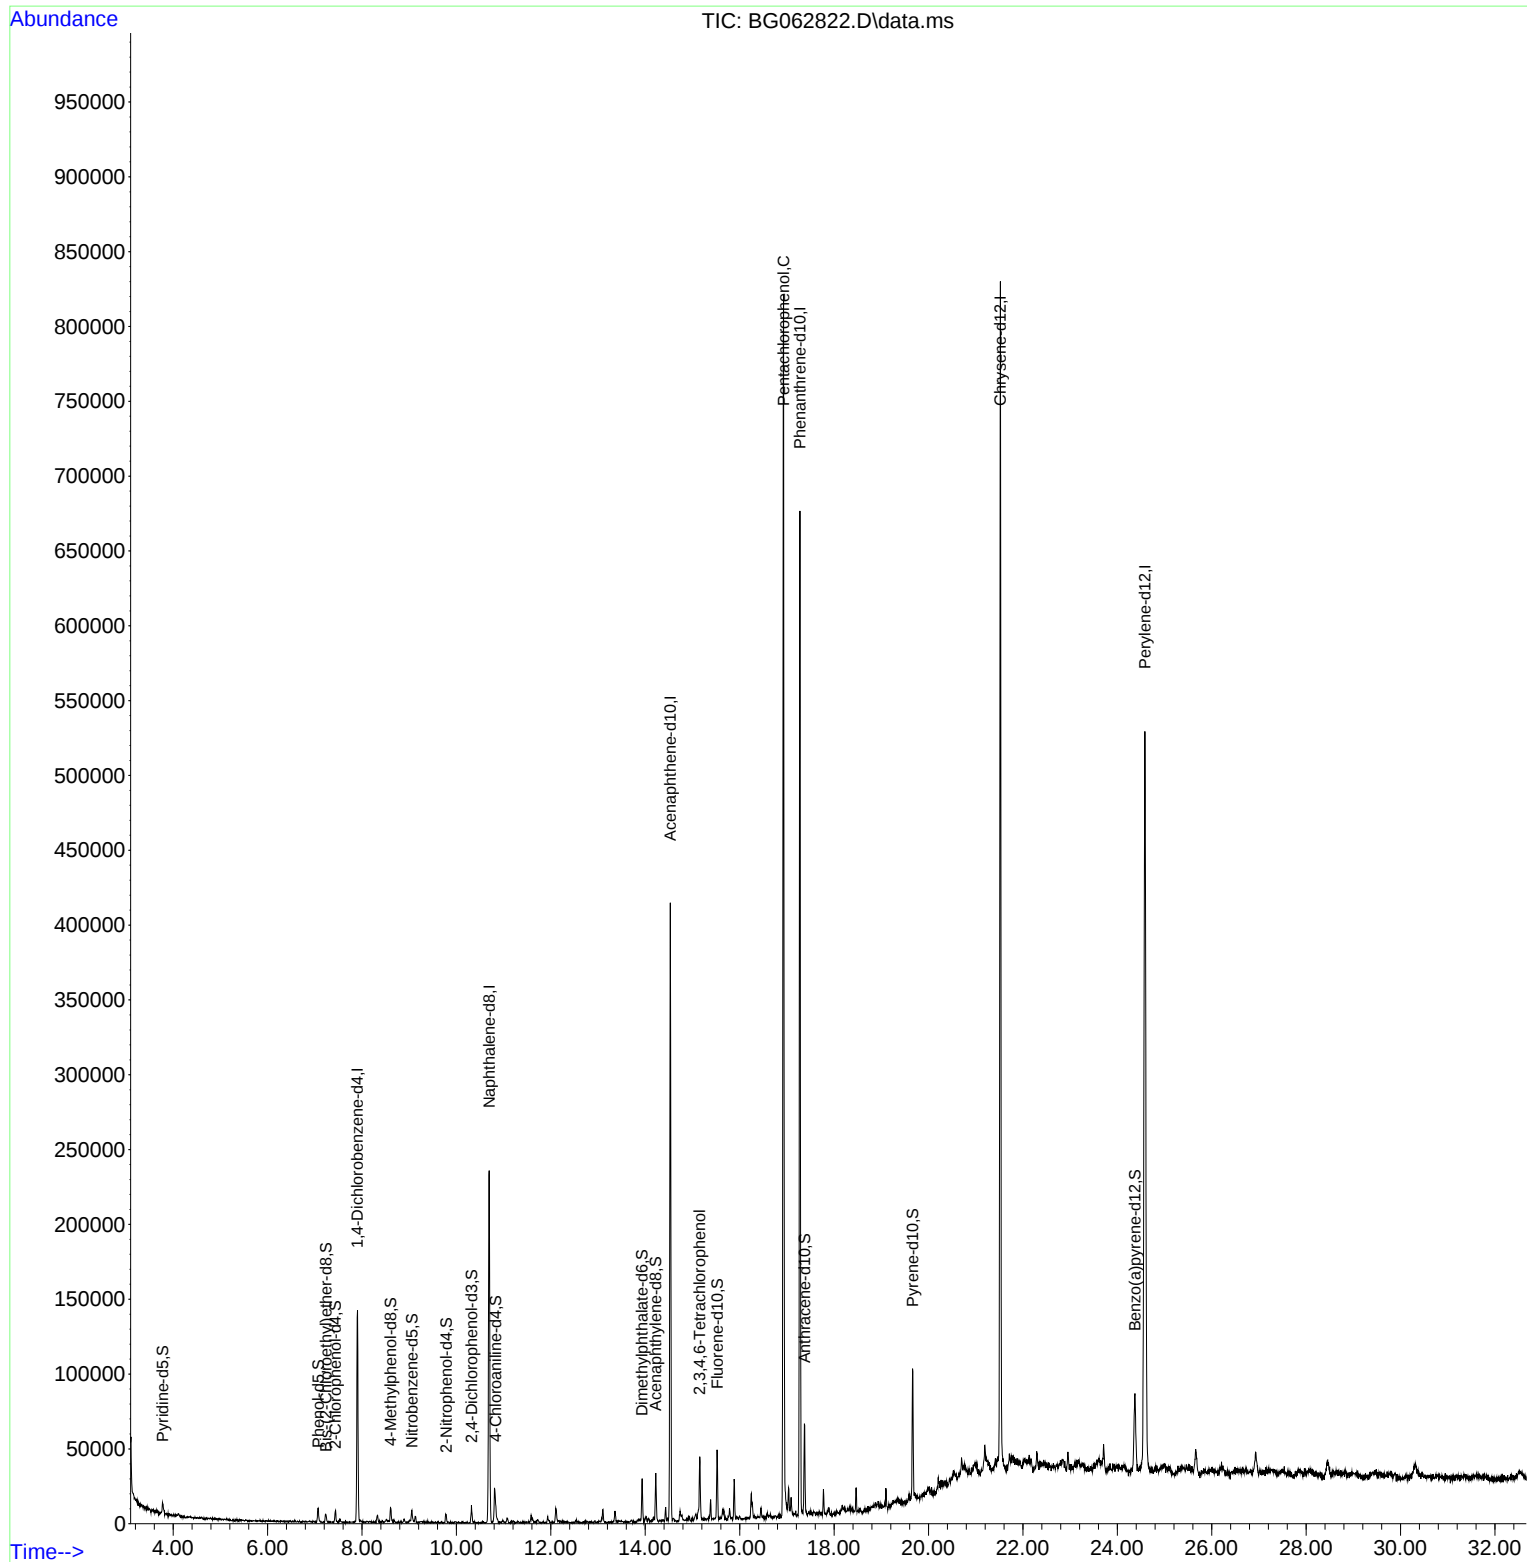




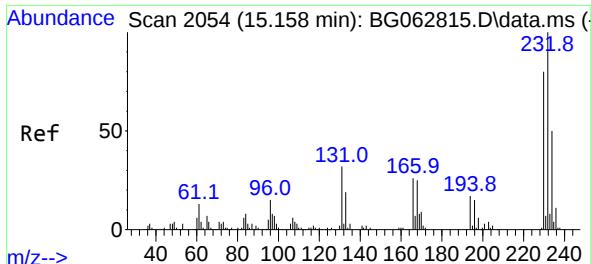


#58
2,3,4,6-Tetrachlorophenol
Concen: 2.934 ng/ul
RT: 15.154 min Scan# 2054
Delta R.T. -0.001 min
Lab File: BG062822.D
Acq: 14 Sep 2024 21:57

Instrument :
BNA_G
ClientSampleId :
DDC57DL

Tgt Ion:232 Resp: 9930

Ion	Ratio	Lower	Upper
232	100		
131	29.8	26.6	40.0
130	0.0	1.6	2.4#
166	26.8	20.6	31.0

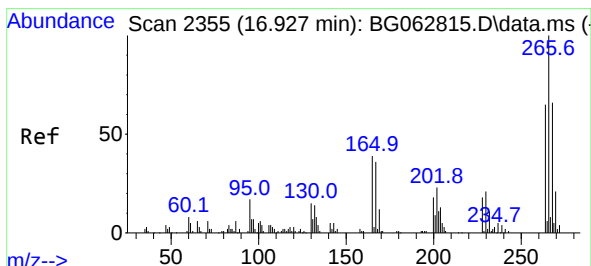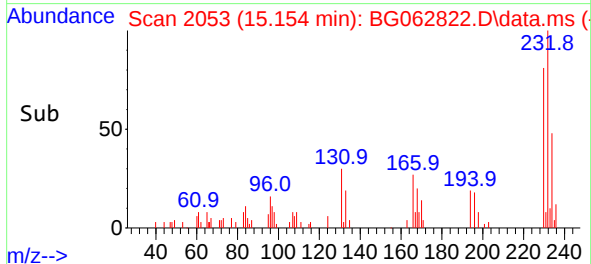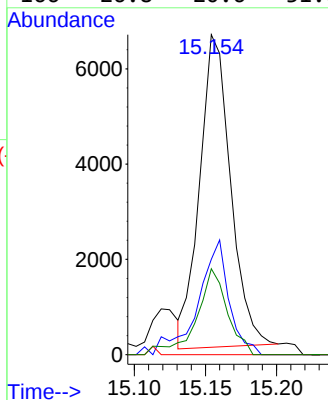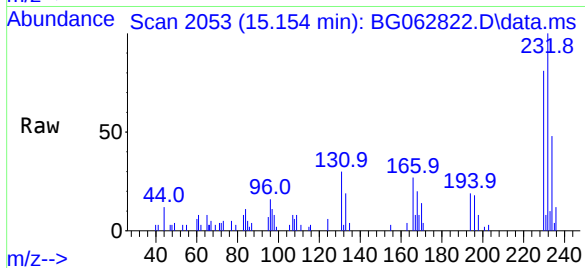

#71
Pentachlorophenol
Concen: 51.894 ng/ul
RT: 16.929 min Scan# 2355
Delta R.T. -0.001 min
Lab File: BG062822.D
Acq: 14 Sep 2024 21:57

Tgt Ion:266 Resp: 171402

Ion	Ratio	Lower	Upper
266	100		
264	62.4	48.6	72.8
268	68.8	49.5	74.3

