

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062824.D
 Acq On : 14 Sep 2024 23:16
 Operator : JU/RC
 Sample : P3898-15DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC88DL

Quant Time: Sep 15 01:40:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	46446	20.000	ng/ul	0.00
20) Naphthalene-d8	10.691	136	185191	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	154973	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.277	188	424660	20.000	ng/ul	0.00
79) Chrysene-d12	21.519	240	498966	20.000	ng/ul	0.00
88) Perylene-d12	24.580	264	560360	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.072	99	5032	1.236	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.230	67	2867	1.174	ng/ul	0.00
11) 2-Chlorophenol-d4	7.436	132	3939	1.328	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	4357	1.284	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	1939	1.465	ng/ul	0.00
24) 2-Nitrophenol-d4	9.780	143	2074	1.433	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.321	165	4537	1.439	ng/ul	0.00
31) 4-Chloroaniline-d4	10.826	131	4994	1.152	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	17717	1.485	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	19328	1.458	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	2204	1.087	ng/ul	0.00
60) Fluorene-d10	15.520	176	16737	1.556	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.638	200	1899	0.777	ng/ul	0.00
73) Anthracene-d10	17.371	188	32387	1.616	ng/ul	0.00
81) Pyrene-d10	19.663	212	43493	1.549	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.369	264	46734	1.579	ng/ul	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.156	232	12327	3.511	ng/ul#	93
71) Pentachlorophenol	16.925	266	112241	33.633	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062824.D
Acq On : 14 Sep 2024 23:16
Operator : JU/RC
Sample : P3898-15DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC88DL

Quant Time: Sep 15 01:40:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration




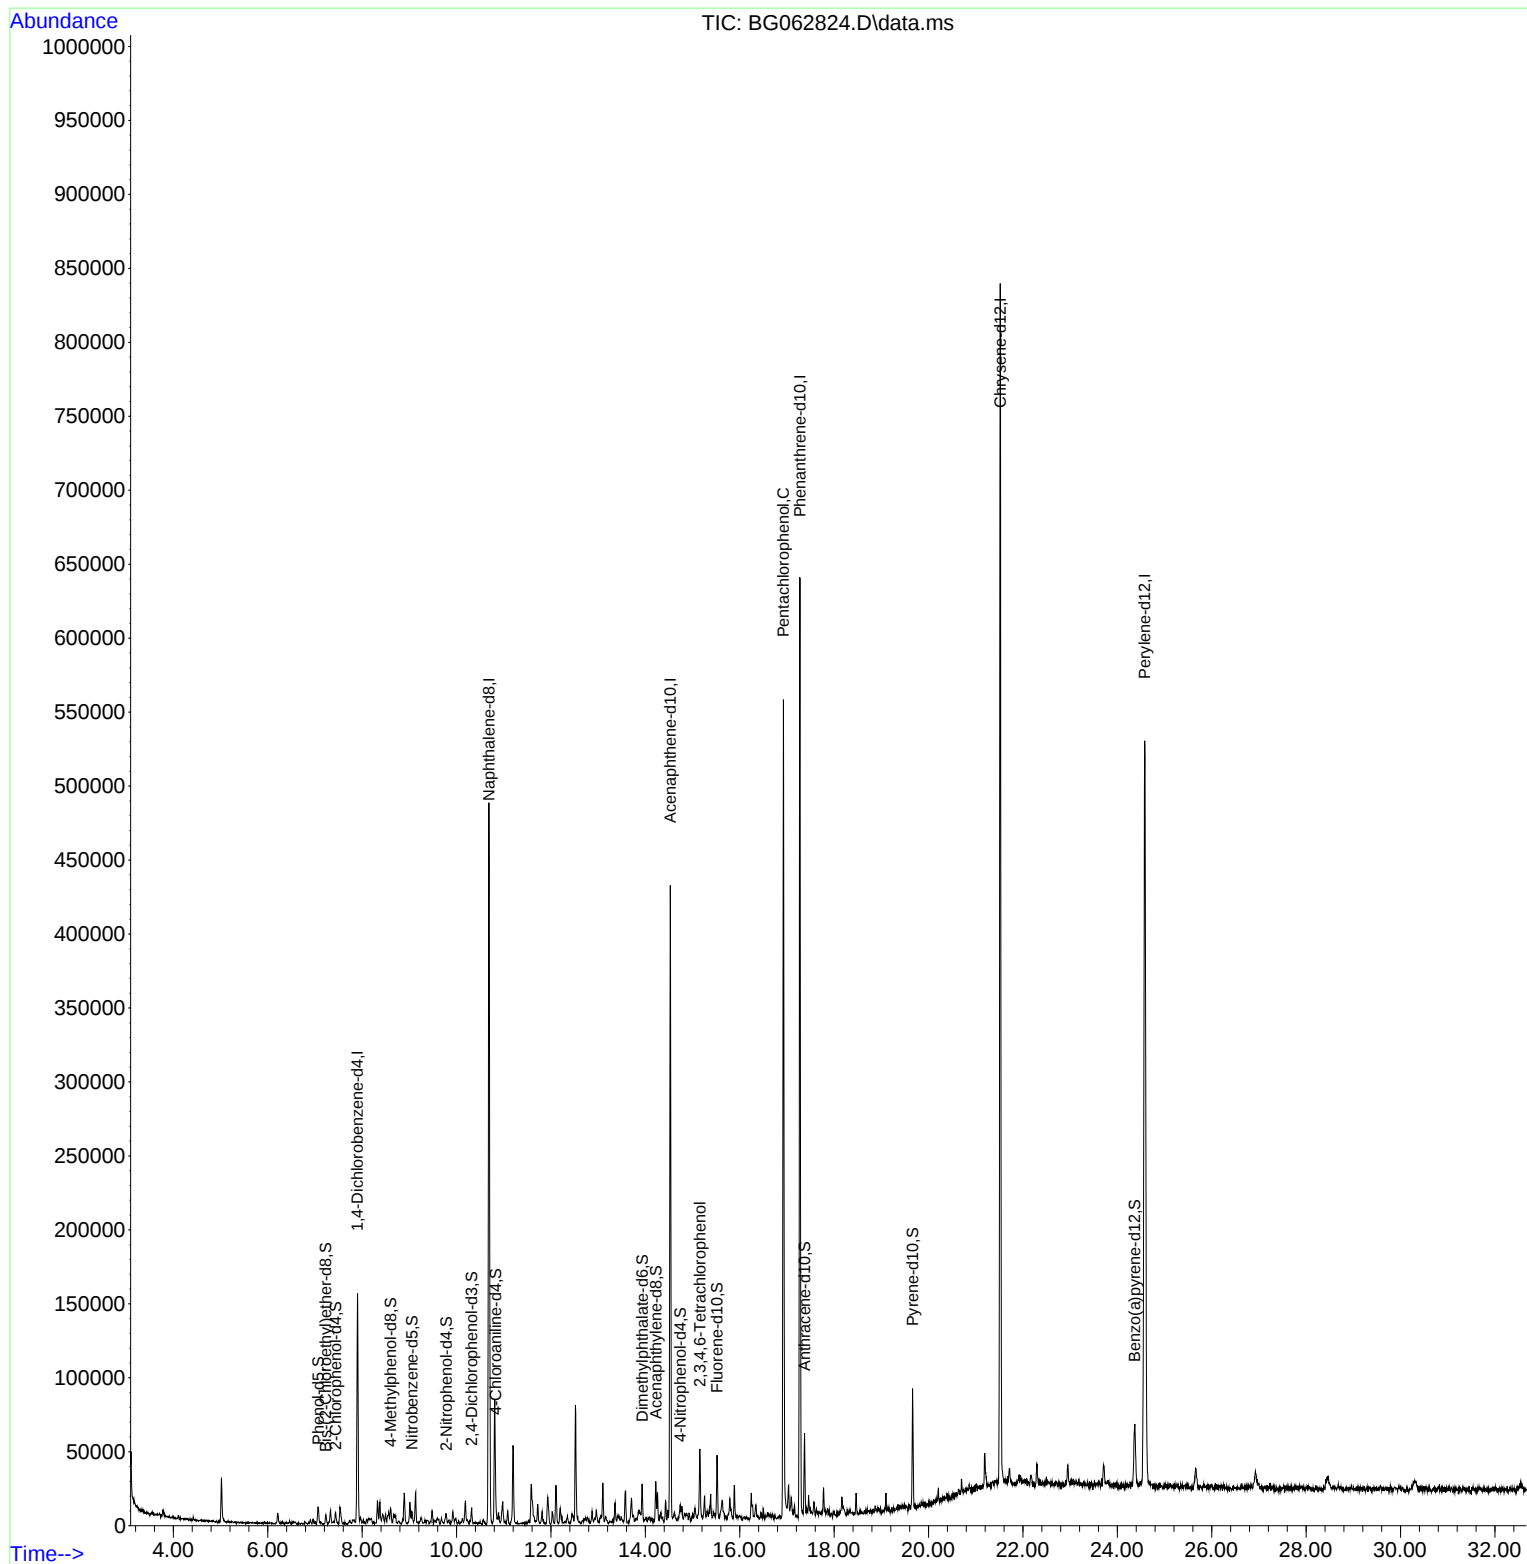


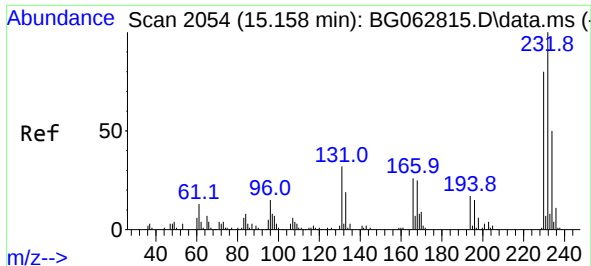

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.511 ng/ul
RT: 15.156 min Scan# 2054
Delta R.T. 0.001 min
Lab File: BG062824.D
Acq: 14 Sep 2024 23:16

Instrument :
BNA_G
ClientSampleId :
DDC88DL

Tgt Ion:	232	Resp:	12327
Ion Ratio	Lower	Upper	
232	100		
131	28.8	26.6	40.0
130	4.2	1.6	2.4#
166	22.7	20.6	31.0

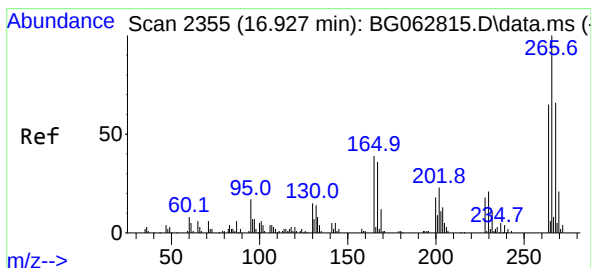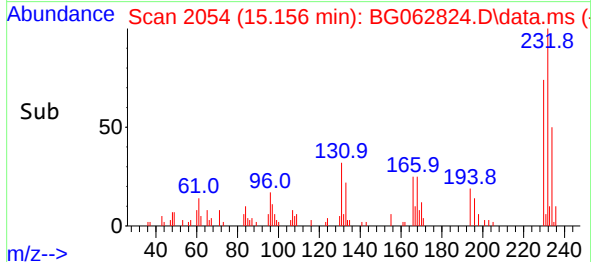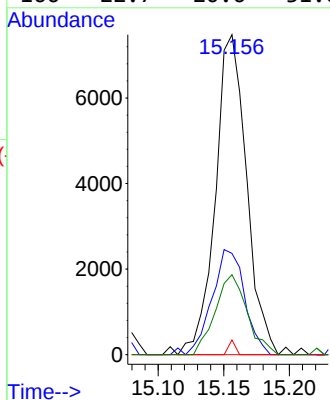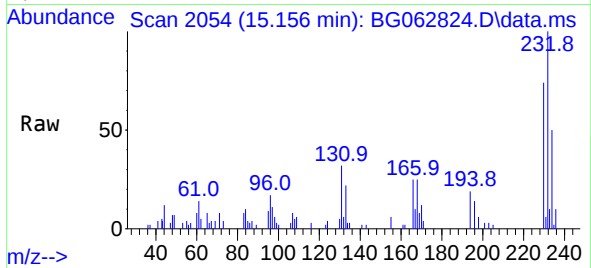

#71
Pentachlorophenol
Concen: 33.633 ng/ul
RT: 16.925 min Scan# 2355
Delta R.T. -0.005 min
Lab File: BG062824.D
Acq: 14 Sep 2024 23:16

Tgt Ion:	266	Resp:	112241
Ion Ratio	Lower	Upper	
266	100		
264	65.1	48.6	72.8
268	66.8	49.5	74.3

