

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062885.D
 Acq On : 16 Sep 2024 18:51
 Operator : JU/RC
 Sample : P3899-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC56

Quant Time: Sep 17 01:28:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	36634	20.000	ng/u1	0.00
20) Naphthalene-d8	10.690	136	141494	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.527	164	124783	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.276	188	359920	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.524	240	434928	20.000	ng/u1	# 0.00
88) Perylene-d12	24.585	264	490754	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	2115	2.610	ng/uL	0.00
4) Pyridine-d5	3.769	84	31882	12.359	ng/u1	0.00
7) Phenol-d5	7.071	99	45466	14.153	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.229	67	24530	12.737	ng/u1	0.00
11) 2-Chlorophenol-d4	7.435	132	36010	15.390	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	40663	15.190	ng/u1	0.00
21) Nitrobenzene-d5	9.051	128	18262	18.058	ng/u1	0.00
24) 2-Nitrophenol-d4	9.773	143	23157	20.938	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.314	165	43414	18.025	ng/u1	0.00
31) 4-Chloroaniline-d4	10.825	131	53679	16.214	ng/u1	0.00
46) Dimethylphthalate-d6	13.933	166	174823	18.193	ng/u1	0.00
49) Acenaphthylene-d8	14.221	160	190573	17.857	ng/u1	0.00
54) 4-Nitrophenol-d4	14.732	143	20737	12.704	ng/u1	0.00
60) Fluorene-d10	15.519	176	161277	18.625	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.637	200	26771	12.931	ng/u1	0.00
73) Anthracene-d10	17.370	188	314583	18.520	ng/u1	0.00
81) Pyrene-d10	19.662	212	446446	18.241	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.374	264	498913	19.253	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.930	266	6798	2.403	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062885.D
Acq On : 16 Sep 2024 18:51
Operator : JU/RC
Sample : P3899-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC56

Quant Time: Sep 17 01:28:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration

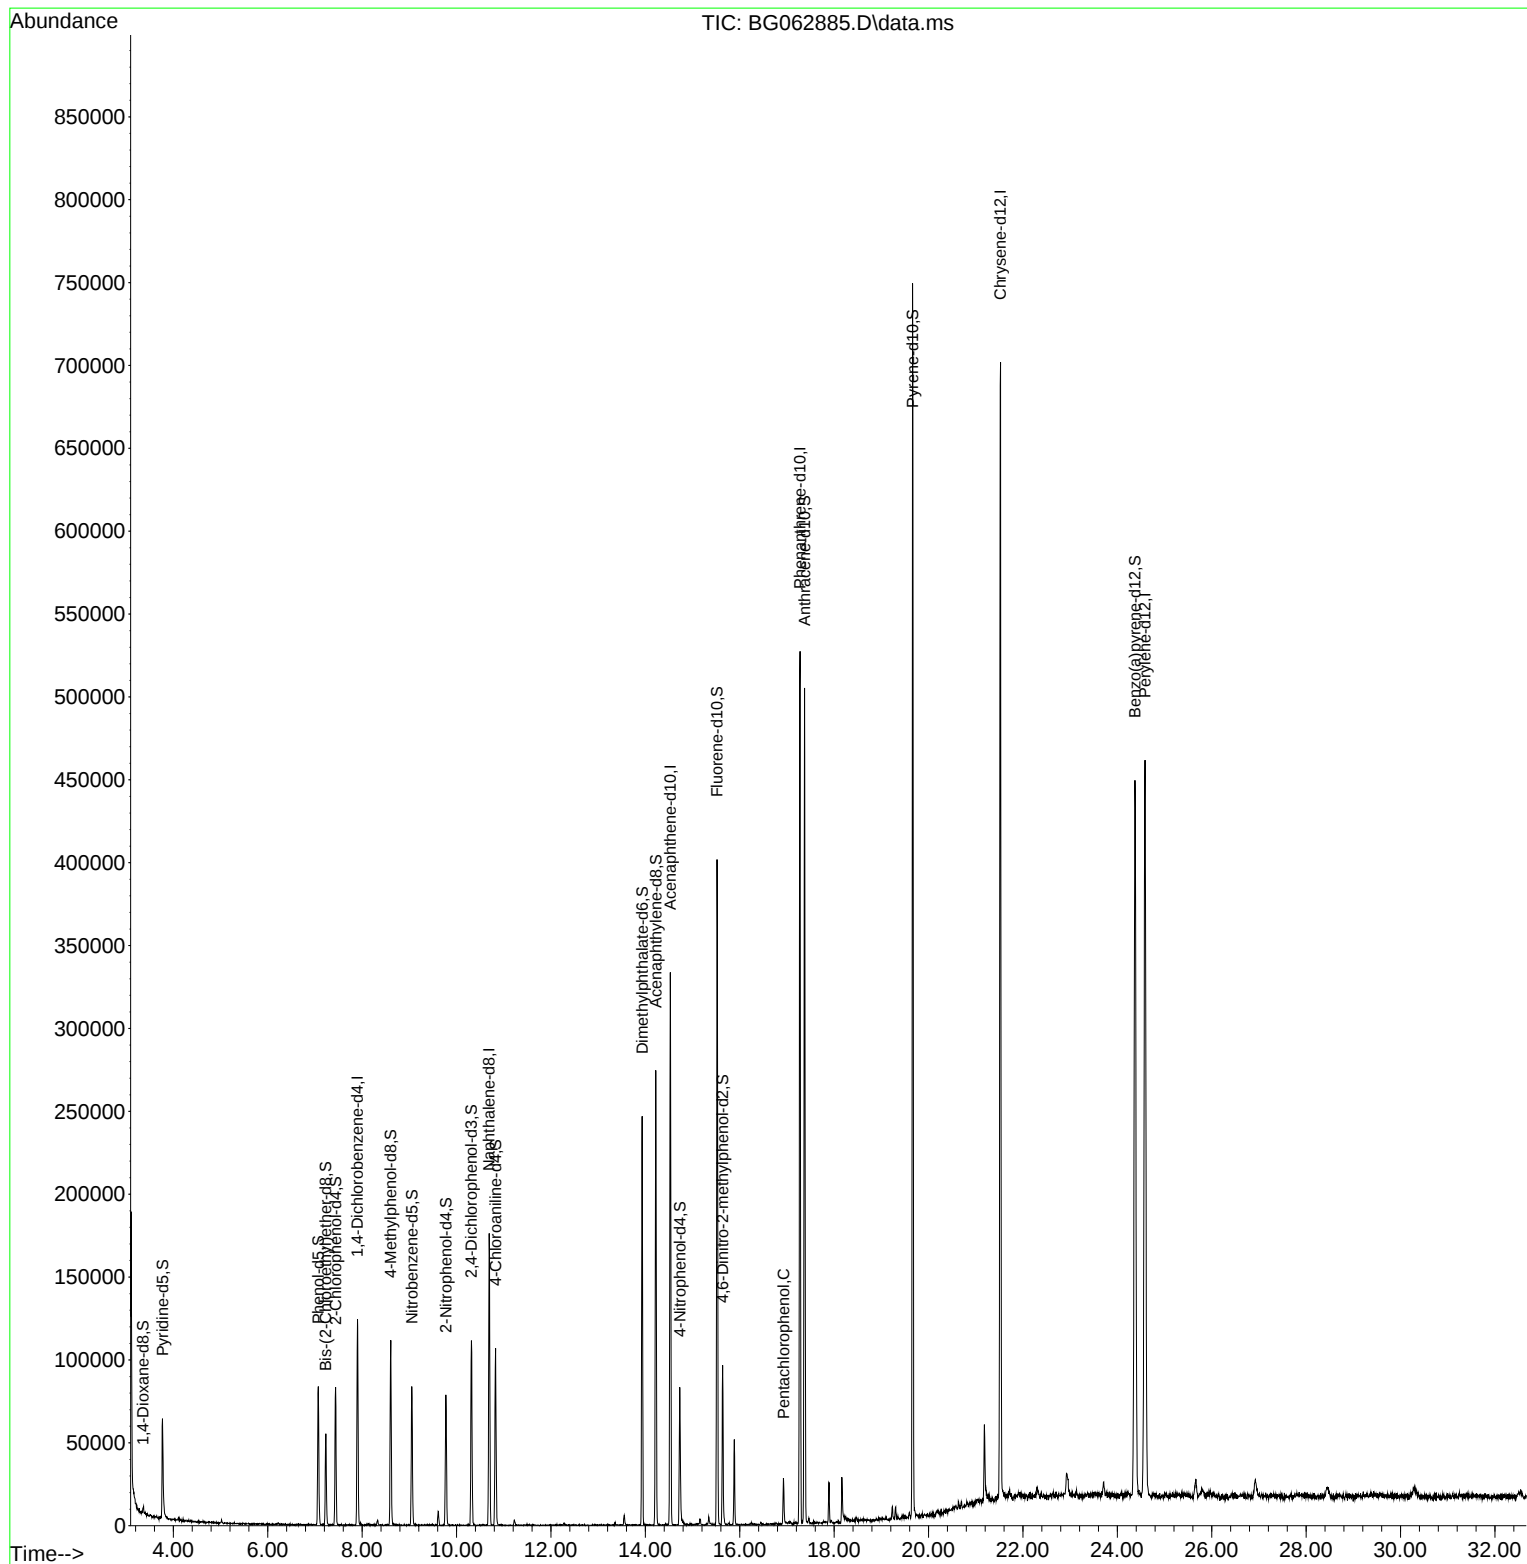

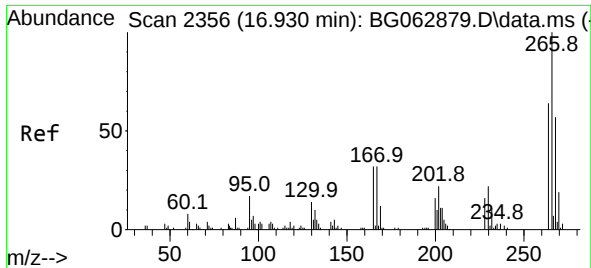

#71
 Pentachlorophenol
 Concen: 2.403 ng/ul
 RT: 16.930 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BG062885.D
 Acq: 16 Sep 2024 18:51

Instrument :
 BNA_G
 ClientSampleId :
 DDC56

Tgt Ion:266 Resp: 6798
 Ion Ratio Lower Upper
 266 100
 264 72.0 48.6 72.8
 268 60.5 49.5 74.3

