

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062790.D
 Acq On : 13 Sep 2024 16:21
 Operator : JU/RC
 Sample : PB163308BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK308

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	51	rVB5	14291	19690	0.77%	0.090%
2	3.764	111	115	125	rBV	172208	300298	11.73%	1.373%
3	4.104	170	173	178	rVB4	5443	7508	0.29%	0.034%
4	7.066	670	677	689	rBV	192189	333527	13.03%	1.525%
5	7.230	699	705	720	rVB	145252	242711	9.48%	1.110%
6	7.436	733	740	751	rVB	188369	332656	13.00%	1.521%
7	7.900	811	819	830	rBV	205364	354230	13.84%	1.620%
8	8.599	930	938	947	rBV2	273733	486999	19.03%	2.227%
9	9.052	1007	1015	1023	rBV	209857	366155	14.31%	1.674%
10	9.774	1128	1138	1148	rBV	179405	306696	11.98%	1.403%
11	10.315	1222	1230	1239	rBV	283696	500959	19.57%	2.291%
12	10.374	1239	1240	1250	rVB5	2815	4180	0.16%	0.019%
13	10.691	1287	1294	1302	rBV	318574	572760	22.38%	2.619%
14	10.826	1309	1317	1327	rBV	256276	483759	18.90%	2.212%
15	12.277	1559	1564	1571	rVB4	4252	7783	0.30%	0.036%
16	13.934	1839	1846	1854	rBV	624616	890472	34.79%	4.072%
17	14.222	1887	1895	1903	rBV	679155	1047460	40.93%	4.790%
18	14.528	1940	1947	1954	rBV	616699	943057	36.85%	4.313%
19	14.727	1974	1981	1994	rBV	267397	459371	17.95%	2.101%
20	14.939	2014	2017	2023	rVB4	1503	2828	0.11%	0.013%
21	15.521	2108	2116	2127	rBV	988787	1445923	56.50%	6.612%
22	15.638	2130	2136	2148	rVV	277831	430553	16.82%	1.969%
23	15.761	2152	2157	2161	rVB6	3995	7189	0.28%	0.033%
24	16.308	2246	2250	2256	rBV3	3044	5070	0.20%	0.023%
25	17.271	2407	2414	2424	rBV	948061	1405807	54.93%	6.429%
26	17.371	2424	2431	2443	rVB2	1243365	1838132	71.82%	8.406%
27	17.941	2525	2528	2535	rBV4	4048	5485	0.21%	0.025%
28	18.723	2656	2661	2663	rBV2	1817	2980	0.12%	0.014%
29	19.228	2741	2747	2752	rBV	19486	25510	1.00%	0.117%
30	19.298	2754	2759	2765	rVV	14844	21991	0.86%	0.101%
31	19.592	2805	2809	2814	rBV7	6468	10118	0.40%	0.046%
32	19.663	2814	2821	2834	rVV	1798653	2462861	96.23%	11.263%
33	20.050	2885	2887	2889	rBV	2925	2649	0.10%	0.012%
34	20.174	2906	2908	2910	rBV3	3608	2847	0.11%	0.013%
35	20.397	2942	2946	2948	rBV5	2974	3823	0.15%	0.017%
36	20.632	2983	2986	2991	rBV7	10412	12741	0.50%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062790.D
 Acq On : 13 Sep 2024 16:21
 Operator : JU/RC
 Sample : PB163308BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK308

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	20.967	3041	3043	3045	rBV3	3635	3623	0.14%	0.017%
38	21.519	3130	3137	3147	rBV	1138107	1827110	71.39%	8.355%
39	21.719	3167	3171	3173	rBV5	5542	7321	0.29%	0.033%
40	22.295	3266	3269	3274	rVB7	10730	14424	0.56%	0.066%
41	22.953	3378	3381	3389	rVB8	13517	23682	0.93%	0.108%
42	23.711	3507	3510	3517	rVB7	14687	27435	1.07%	0.125%
43	24.369	3611	3622	3638	rBV2	974826	2559358	100.00%	11.704%
44	24.580	3647	3658	3674	rVB2	707555	1945356	76.01%	8.896%
45	25.068	3739	3741	3743	rVB3	4626	3226	0.13%	0.015%
46	25.662	3836	3842	3848	rBV5	16938	37944	1.48%	0.174%
47	26.931	4053	4058	4067	rVB7	16618	43829	1.71%	0.200%
48	27.189	4100	4102	4103	rBV2	4117	3271	0.13%	0.015%
49	27.459	4145	4148	4150	rBV3	4560	6277	0.25%	0.029%
50	29.392	4476	4477	4479	rBV2	4107	3667	0.14%	0.017%
51	29.780	4541	4543	4544	rBV2	4085	2590	0.10%	0.012%
52	29.886	4560	4561	4564	rBV3	5523	5155	0.20%	0.024%
53	31.096	4765	4767	4768	rBV2	4241	2930	0.11%	0.013%
54	31.320	4804	4805	4807	rBV2	3992	3333	0.13%	0.015%




Sum of corrected areas: 21867309

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062790.D
Acq On : 13 Sep 2024 16:21
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

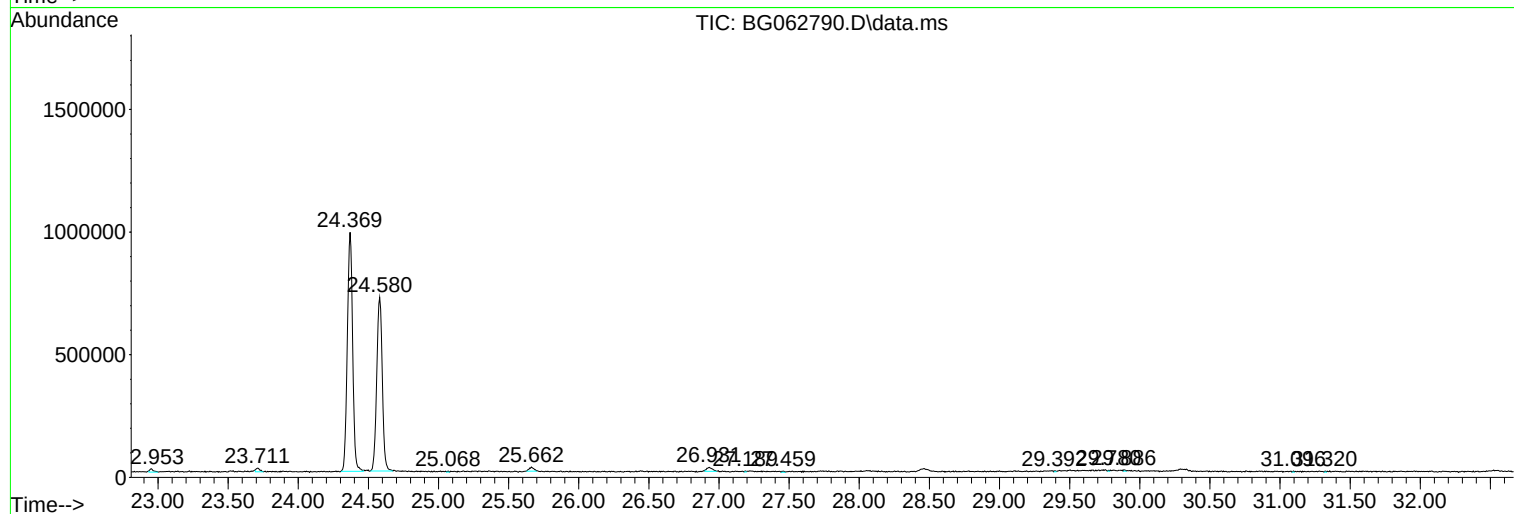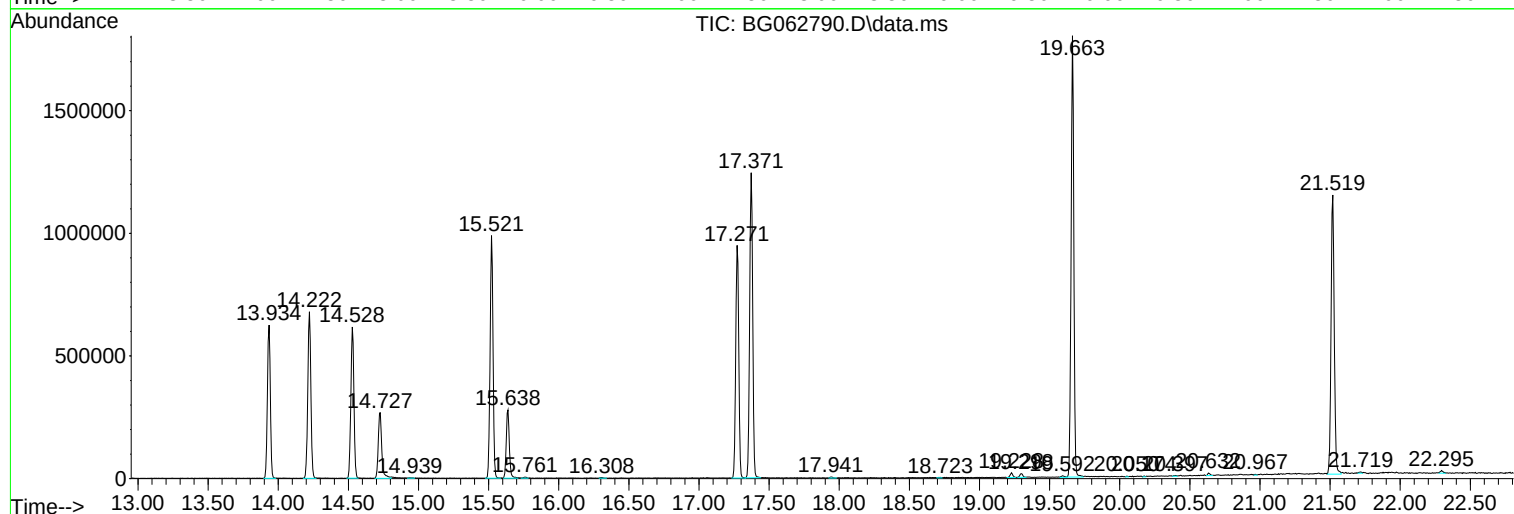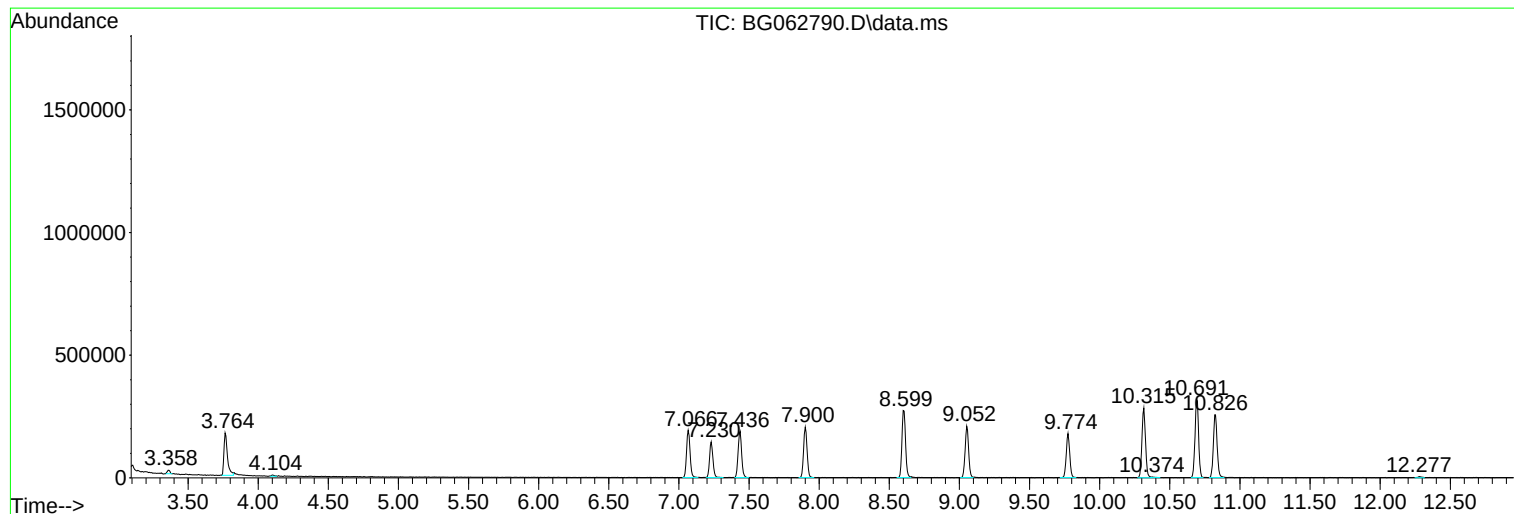

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062790.D
Acq On : 13 Sep 2024 16:21
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062790.D
Acq On : 13 Sep 2024 16:21
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc