

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062822.D
 Acq On : 14 Sep 2024 21:57
 Operator : JU/RC
 Sample : P3898-07DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC57DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.297	33	35	38	rVB2	2661	2430	0.18%	0.032%
2	3.374	46	48	52	rVB5	2315	3051	0.23%	0.041%
3	3.773	113	116	124	rVB5	8632	18091	1.37%	0.241%
4	3.850	124	129	130	rBV3	1277	2354	0.18%	0.031%
5	4.114	170	174	177	rVV5	2346	4182	0.32%	0.056%
6	7.069	670	677	685	rVV3	9561	18181	1.38%	0.243%
7	7.228	700	704	713	rVB5	5695	11640	0.88%	0.155%
8	7.440	733	740	743	rBV2	8170	13492	1.02%	0.180%
9	7.528	752	755	762	rBV4	2292	3483	0.26%	0.046%
10	7.904	812	819	826	rVV	141519	245497	18.59%	3.277%
11	8.327	886	891	897	rBV4	5018	9592	0.73%	0.128%
12	8.515	920	923	928	rVB5	1697	2479	0.19%	0.033%
13	8.603	934	938	943	rBV3	9131	15206	1.15%	0.203%
14	8.891	982	987	995	rVB6	2652	4822	0.37%	0.064%
15	9.055	1010	1015	1021	rVV2	7496	12547	0.95%	0.167%
16	9.126	1023	1027	1031	rVB4	4073	6700	0.51%	0.089%
17	9.772	1134	1137	1143	rBV3	5813	10223	0.77%	0.136%
18	9.978	1166	1172	1179	rBV2	1120	3601	0.27%	0.048%
19	10.319	1225	1230	1236	rBV2	11616	16677	1.26%	0.223%
20	10.695	1280	1294	1302	rBV	235498	449285	34.02%	5.996%
21	10.806	1306	1313	1327	rVB6	23447	57624	4.36%	0.769%
22	10.983	1338	1343	1349	rBV4	2019	3555	0.27%	0.047%
23	11.071	1353	1358	1365	rBV4	3143	6754	0.51%	0.090%
24	11.582	1440	1445	1448	rBV3	5309	8749	0.66%	0.117%
25	11.723	1465	1469	1474	rBV4	2167	4017	0.30%	0.054%
26	11.934	1501	1505	1509	rBV5	4320	6930	0.52%	0.092%
27	12.105	1527	1534	1540	rBV3	9774	19286	1.46%	0.257%
28	12.146	1540	1541	1546	rVV4	1598	2603	0.20%	0.035%
29	12.534	1602	1607	1608	rBV2	1899	2576	0.20%	0.034%
30	12.933	1671	1675	1679	rBV3	1604	2702	0.20%	0.036%
31	13.074	1695	1699	1700	rVV2	2970	3436	0.26%	0.046%
32	13.104	1700	1704	1711	rVV2	8937	14239	1.08%	0.190%
33	13.356	1741	1747	1751	rBV2	7484	11518	0.87%	0.154%
34	13.715	1802	1808	1811	rVB4	1868	3795	0.29%	0.051%
35	13.850	1826	1831	1832	rBV2	1875	2393	0.18%	0.032%
36	13.932	1840	1845	1851	rVB	29331	44516	3.37%	0.594%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062822.D
 Acq On : 14 Sep 2024 21:57
 Operator : JU/RC
 Sample : P3898-07DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC57DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	14.014	1853	1859	1864	rVB4	3862	7587	0.57%	0.101%
38	14.061	1864	1867	1869	rBV3	2046	2747	0.21%	0.037%
39	14.179	1885	1887	1890	rVV3	3021	2716	0.21%	0.036%
40	14.220	1890	1894	1904	rVB	32842	50722	3.84%	0.677%
41	14.431	1925	1930	1935	rBV3	9958	14352	1.09%	0.192%
42	14.473	1935	1937	1940	rVV4	2329	3039	0.23%	0.041%
43	14.531	1940	1947	1954	rVV	413248	631959	47.86%	8.434%
44	14.590	1954	1957	1963	rVB5	1740	3346	0.25%	0.045%
45	14.737	1977	1982	1986	rVV4	6911	12086	0.92%	0.161%
46	14.778	1986	1989	1993	rVB4	3558	4710	0.36%	0.063%
47	14.931	2011	2015	2020	rVB4	3094	4783	0.36%	0.064%
48	15.072	2030	2039	2042	rBV7	4780	11397	0.86%	0.152%
49	15.154	2044	2053	2060	rVB2	41904	75502	5.72%	1.008%
50	15.354	2084	2087	2088	rBV	2724	2491	0.19%	0.033%
51	15.383	2088	2092	2096	rVB	13607	16868	1.28%	0.225%
52	15.518	2110	2115	2121	rVB	46754	71219	5.39%	0.951%
53	15.642	2131	2136	2139	rBV5	6447	11397	0.86%	0.152%
54	15.783	2157	2160	2164	rVB3	6657	8298	0.63%	0.111%
55	15.883	2172	2177	2182	rBV	27158	38588	2.92%	0.515%
56	15.936	2184	2186	2191	rVV4	2259	3276	0.25%	0.044%
57	15.994	2193	2196	2205	rVB4	2621	5275	0.40%	0.070%
58	16.247	2232	2239	2241	rBV2	17332	25868	1.96%	0.345%
59	16.453	2270	2274	2279	rVV3	6732	9367	0.71%	0.125%
60	16.500	2279	2282	2285	rVB3	1871	2537	0.19%	0.034%
61	16.746	2321	2324	2330	rVB5	1896	3731	0.28%	0.050%
62	16.817	2333	2336	2339	rVB4	2707	3681	0.28%	0.049%
63	16.840	2339	2340	2346	rBV5	2509	4317	0.33%	0.058%
64	16.929	2348	2355	2365	rBV	815786	1261645	95.54%	16.839%
65	17.034	2370	2373	2378	rVV2	18806	29768	2.25%	0.397%
66	17.087	2378	2382	2387	rVV3	12288	18926	1.43%	0.253%
67	17.275	2407	2414	2420	rBV	671677	967544	73.27%	12.913%
68	17.316	2420	2421	2425	rVV3	3571	4278	0.32%	0.057%
69	17.369	2425	2430	2437	rVV	60928	95271	7.21%	1.272%
70	17.563	2460	2463	2468	rBV6	2982	5915	0.45%	0.079%
71	17.775	2495	2499	2505	rBV2	17740	23497	1.78%	0.314%
72	17.857	2510	2513	2514	rBV2	2691	2640	0.20%	0.035%
73	17.886	2516	2518	2523	rVB4	5032	6584	0.50%	0.088%
74	17.998	2531	2537	2538	rBV5	2500	3836	0.29%	0.051%
75	18.051	2544	2546	2549	rBV4	3085	3697	0.28%	0.049%
76	18.174	2563	2567	2568	rBV4	3813	4498	0.34%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062822.D
 Acq On : 14 Sep 2024 21:57
 Operator : JU/RC
 Sample : P3898-07DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC57DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

77	18.333	2591	2594	2597	rVB4	3867	4272	0.32%	0.057%
78	18.468	2612	2617	2620	rVB3	16208	20552	1.56%	0.274%
79	18.538	2626	2629	2631	rBV4	2984	3263	0.25%	0.044%
80	18.791	2669	2672	2674	rBV4	2073	3123	0.24%	0.042%
81	18.932	2694	2696	2699	rVB4	4143	3601	0.27%	0.048%
82	19.020	2708	2711	2713	rBV4	2592	3379	0.26%	0.045%
83	19.097	2721	2724	2728	rVV2	12376	13966	1.06%	0.186%
84	19.332	2762	2764	2766	rBV3	2550	2439	0.18%	0.033%
85	19.525	2795	2797	2799	rVB3	2903	2409	0.18%	0.032%
86	19.661	2815	2820	2826	rBV	86931	137272	10.40%	1.832%
87	19.919	2862	2864	2865	rBV2	3275	2498	0.19%	0.033%
88	20.066	2887	2889	2891	rVB3	5920	4104	0.31%	0.055%
89	20.207	2911	2913	2914	rBV2	7199	5987	0.45%	0.080%
90	20.266	2921	2923	2924	rBV2	6371	4637	0.35%	0.062%
91	20.301	2927	2929	2933	rVV5	4502	5437	0.41%	0.073%
92	20.701	2995	2997	3001	rVB5	8442	9595	0.73%	0.128%
93	21.194	3078	3081	3084	rVB4	10743	13129	0.99%	0.175%
94	21.523	3130	3137	3149	rVB	791629	1248117	94.52%	16.658%
95	23.709	3507	3509	3516	rVB7	18255	27008	2.05%	0.360%
96	24.373	3615	3622	3630	rVB	51796	136013	10.30%	1.815%
97	24.584	3648	3658	3670	rVB	490385	1320492	100.00%	17.624%
98	27.140	4091	4093	4094	rBV2	5895	3970	0.30%	0.053%
99	27.963	4231	4233	4235	rBV3	5464	5195	0.39%	0.069%
100	32.152	4944	4946	4948	rBV3	5621	3970	0.30%	0.053%




Sum of corrected areas: 7492612

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062822.D
Acq On : 14 Sep 2024 21:57
Operator : JU/RC
Sample : P3898-07DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC57DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

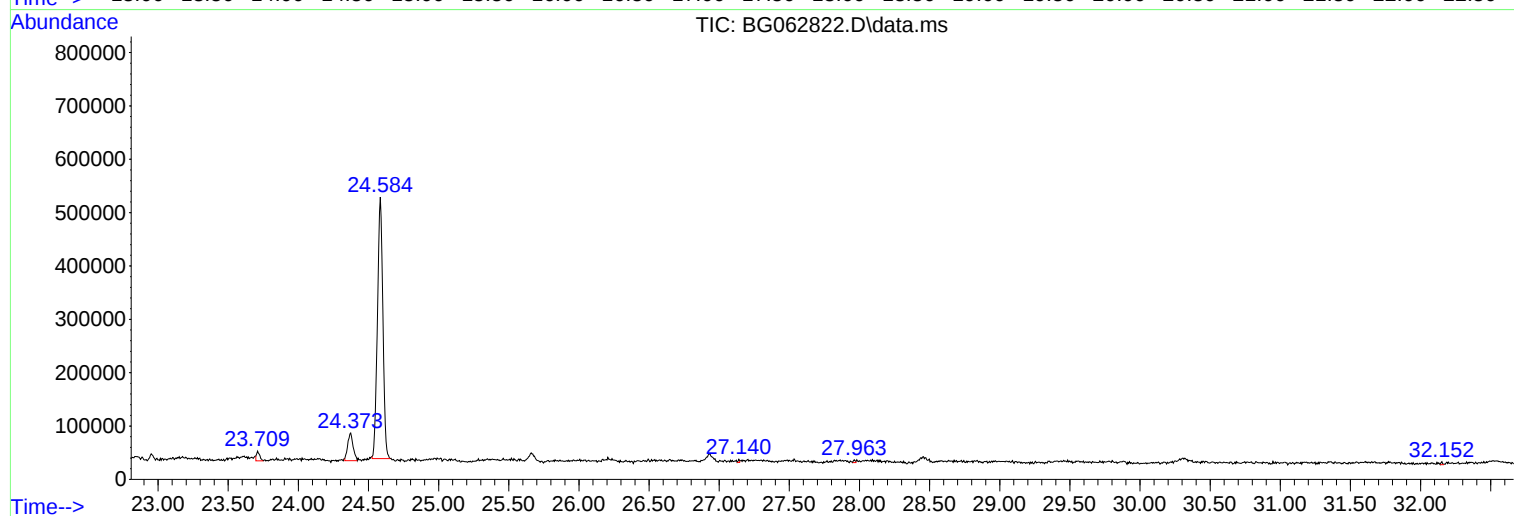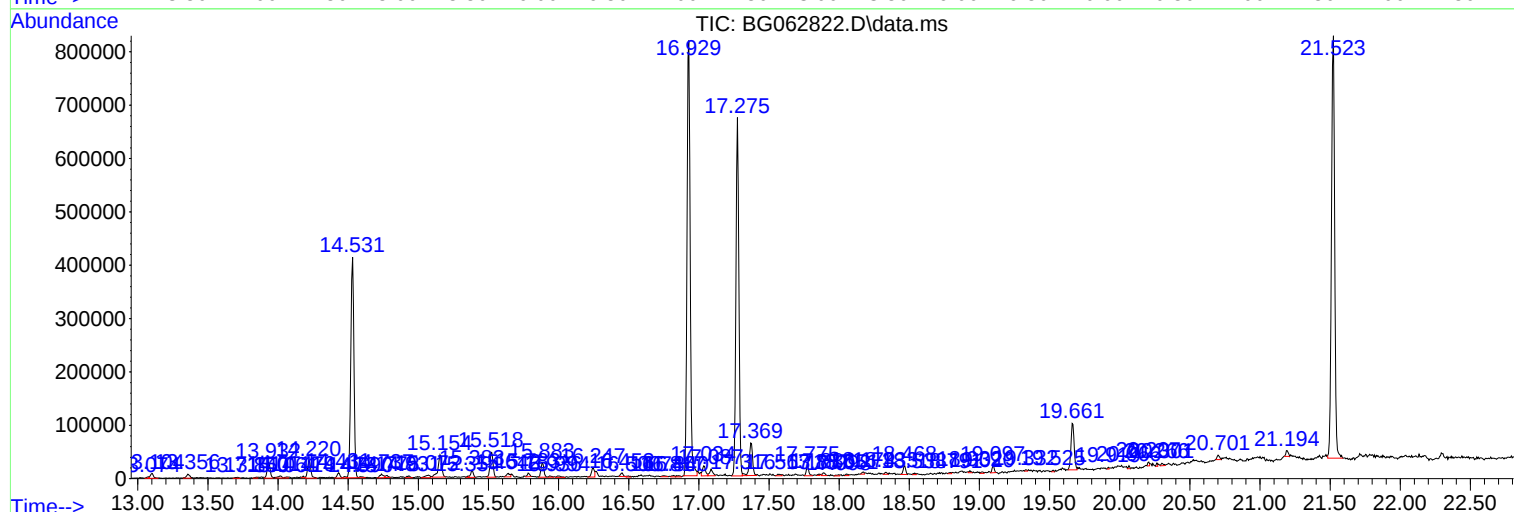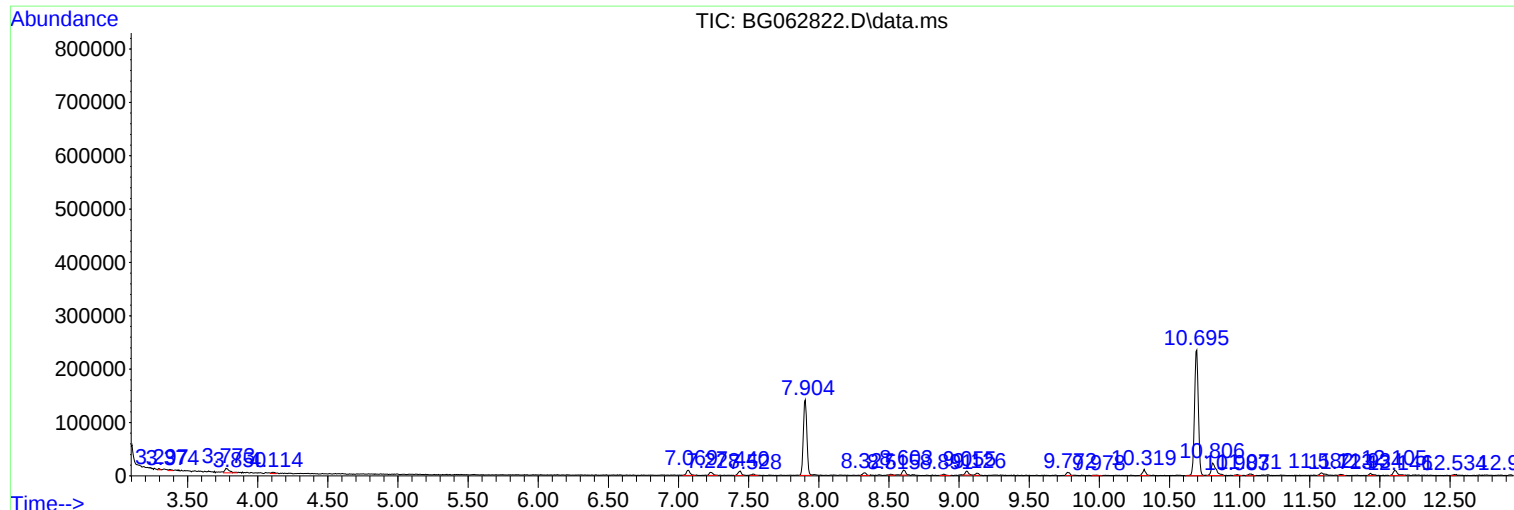

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062822.D
Acq On : 14 Sep 2024 21:57
Operator : JU/RC
Sample : P3898-07DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC57DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062822.D
Acq On : 14 Sep 2024 21:57
Operator : JU/RC
Sample : P3898-07DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC57DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc