

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062887.D
 Acq On : 16 Sep 2024 20:10
 Operator : JU/RC
 Sample : P3899-11DL 20X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC12DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.913	138	140	143	rVB3	1382	1300	0.14%	0.032%
2	3.990	149	153	156	rBV3	1624	2536	0.27%	0.063%
3	4.360	214	216	222	rVB3	2449	3106	0.33%	0.077%
4	5.018	322	328	332	rBV4	1254	2219	0.23%	0.055%
5	5.929	481	483	488	rVB3	1523	1719	0.18%	0.043%
6	6.692	610	613	617	rBV2	740	1187	0.13%	0.029%
7	6.957	652	658	662	rBV2	1167	2053	0.22%	0.051%
8	7.062	672	676	685	rVB3	6068	10570	1.12%	0.261%
9	7.227	700	704	709	rVB	3786	5354	0.57%	0.132%
10	7.327	718	721	725	rVB2	1429	1905	0.20%	0.047%
11	7.433	733	739	747	rVB3	5201	8987	0.95%	0.222%
12	7.527	751	755	763	rVB5	5764	11852	1.25%	0.293%
13	7.903	810	819	825	rBV	91355	154948	16.38%	3.833%
14	8.014	833	838	843	rBV2	1297	2278	0.24%	0.056%
15	8.326	885	891	896	rBV3	2363	3653	0.39%	0.090%
16	8.426	906	908	910	rBV	990	1277	0.14%	0.032%
17	8.496	916	920	922	rBV	821	1150	0.12%	0.028%
18	8.531	923	926	930	rBV2	1405	1850	0.20%	0.046%
19	8.608	934	939	946	rVB4	4723	8226	0.87%	0.204%
20	8.672	946	950	953	rBV2	1380	2359	0.25%	0.058%
21	9.054	1010	1015	1022	rVV2	5257	8709	0.92%	0.215%
22	9.131	1022	1028	1034	rVV4	5445	9103	0.96%	0.225%
23	9.195	1037	1039	1043	rVB	1286	1551	0.16%	0.038%
24	9.777	1134	1138	1143	rBV2	4197	5550	0.59%	0.137%
25	10.317	1225	1230	1235	rBV2	4680	7293	0.77%	0.180%
26	10.694	1286	1294	1304	rVB	123265	221832	23.45%	5.488%
27	10.829	1312	1317	1325	rBV	5599	9250	0.98%	0.229%
28	12.115	1528	1536	1542	rVB3	1519	2552	0.27%	0.063%
29	12.356	1574	1577	1580	rVB2	1349	1467	0.16%	0.036%
30	12.574	1610	1614	1620	rVB2	851	1398	0.15%	0.035%
31	13.355	1743	1747	1753	rVB3	2867	3940	0.42%	0.097%
32	13.849	1826	1831	1835	rVB	1321	2075	0.22%	0.051%
33	13.931	1835	1845	1850	rBV	16810	23913	2.53%	0.592%
34	14.219	1888	1894	1903	rVB3	15798	25680	2.71%	0.635%
35	14.424	1925	1929	1933	rBV2	3470	4023	0.43%	0.100%
36	14.524	1939	1946	1955	rBV	253181	393565	41.61%	9.736%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
 Data File : BG062887.D
 Acq On : 16 Sep 2024 20:10
 Operator : JU/RC
 Sample : P3899-11DL 20X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC12DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Title : SVOA CALIBRATION

37	14.612	1959	1961	1965	rVB	2284	1463	0.15%	0.036%
38	14.736	1979	1982	1993	rBV4	3073	7258	0.77%	0.180%
39	14.918	2011	2013	2016	rBV	916	1172	0.12%	0.029%
40	15.006	2025	2028	2031	rVB2	989	1095	0.12%	0.027%
41	15.153	2048	2053	2058	rBV2	11837	18167	1.92%	0.449%
42	15.347	2082	2086	2089	rBV3	4342	5837	0.62%	0.144%
43	15.376	2089	2091	2096	rVB2	3833	4462	0.47%	0.110%
44	15.517	2108	2115	2122	rBV2	26934	41398	4.38%	1.024%
45	15.641	2129	2136	2139	rBV3	3057	4278	0.45%	0.106%
46	15.793	2156	2162	2164	rVB2	1694	2037	0.22%	0.050%
47	15.887	2173	2178	2182	rBV	2504	4089	0.43%	0.101%
48	16.240	2233	2238	2246	rBV3	4605	9504	1.00%	0.235%
49	16.922	2348	2354	2366	rBV	152349	237406	25.10%	5.873%
50	17.033	2369	2373	2378	rVV4	5085	8959	0.95%	0.222%
51	17.086	2380	2382	2388	rVB4	2629	3858	0.41%	0.095%
52	17.274	2406	2414	2422	rBV	452105	652956	69.03%	16.153%
53	17.368	2425	2430	2438	rVB	36636	54437	5.76%	1.347%
54	17.574	2462	2465	2469	rVB	1292	1838	0.19%	0.045%
55	17.773	2495	2499	2502	rVB	4457	5270	0.56%	0.130%
56	17.850	2510	2512	2516	rBV2	1152	1264	0.13%	0.031%
57	17.891	2516	2519	2523	rVV3	1893	2989	0.32%	0.074%
58	17.944	2526	2528	2533	rVB2	948	1208	0.13%	0.030%
59	18.108	2552	2556	2560	rVB2	782	1173	0.12%	0.029%
60	18.149	2560	2563	2565	rBV	1478	1672	0.18%	0.041%
61	18.385	2599	2603	2606	rBV2	1019	1451	0.15%	0.036%
62	18.467	2613	2617	2621	rVB3	4422	5802	0.61%	0.144%
63	18.866	2682	2685	2687	rBV2	2023	2377	0.25%	0.059%
64	19.031	2711	2713	2715	rBV	1317	1282	0.14%	0.032%
65	19.095	2721	2724	2727	rVB3	3849	3856	0.41%	0.095%
66	19.172	2735	2737	2740	rBV2	978	1114	0.12%	0.028%
67	19.336	2763	2765	2767	rBV3	1181	1199	0.13%	0.030%
68	19.595	2806	2809	2811	rVB3	3138	2861	0.30%	0.071%
69	19.659	2815	2820	2826	rBV	52761	76980	8.14%	1.904%
70	19.818	2845	2847	2849	rBV2	1423	1580	0.17%	0.039%
71	19.900	2859	2861	2864	rBV3	1524	1481	0.16%	0.037%
72	20.200	2910	2912	2916	rVB3	2904	3081	0.33%	0.076%
73	21.187	3077	3080	3084	rBV6	8595	12715	1.34%	0.315%
74	21.516	3130	3136	3146	rBV	552787	881920	93.24%	21.818%
75	24.366	3616	3621	3632	rVB	30315	74452	7.87%	1.842%
76	24.583	3648	3658	3673	rVB2	342837	945858	100.00%	23.399%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062887.D
Acq On : 16 Sep 2024 20:10
Operator : JU/RC
Sample : P3899-11DL 20X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC12DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 4042229

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062887.D
Acq On : 16 Sep 2024 20:10
Operator : JU/RC
Sample : P3899-11DL 20X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC12DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

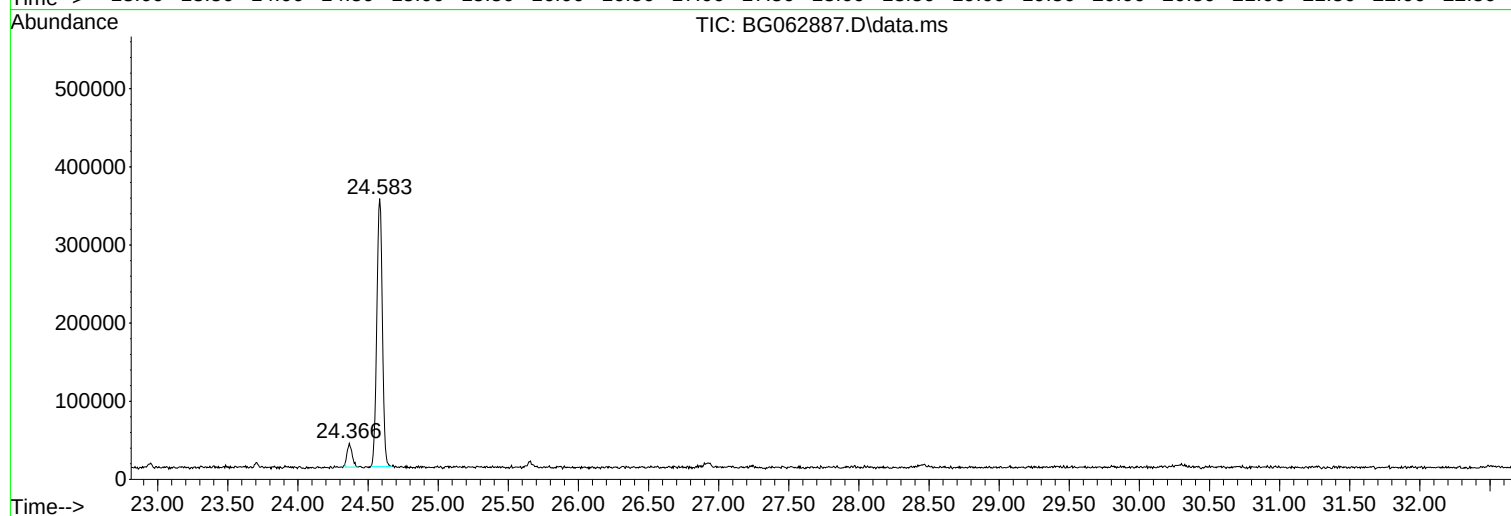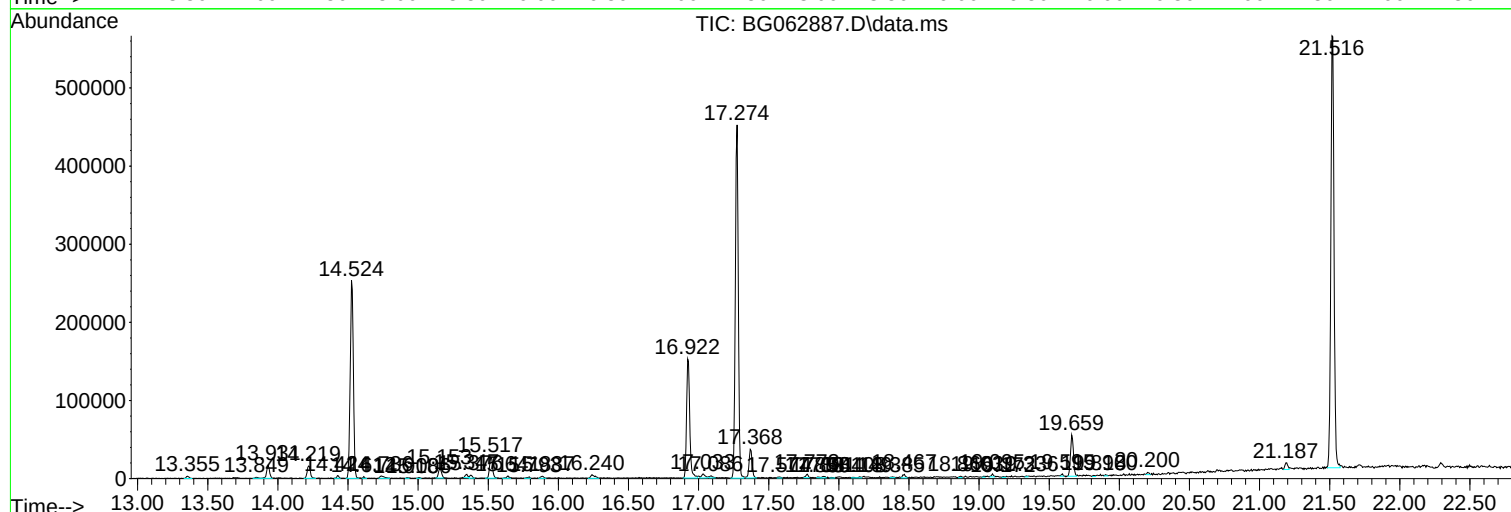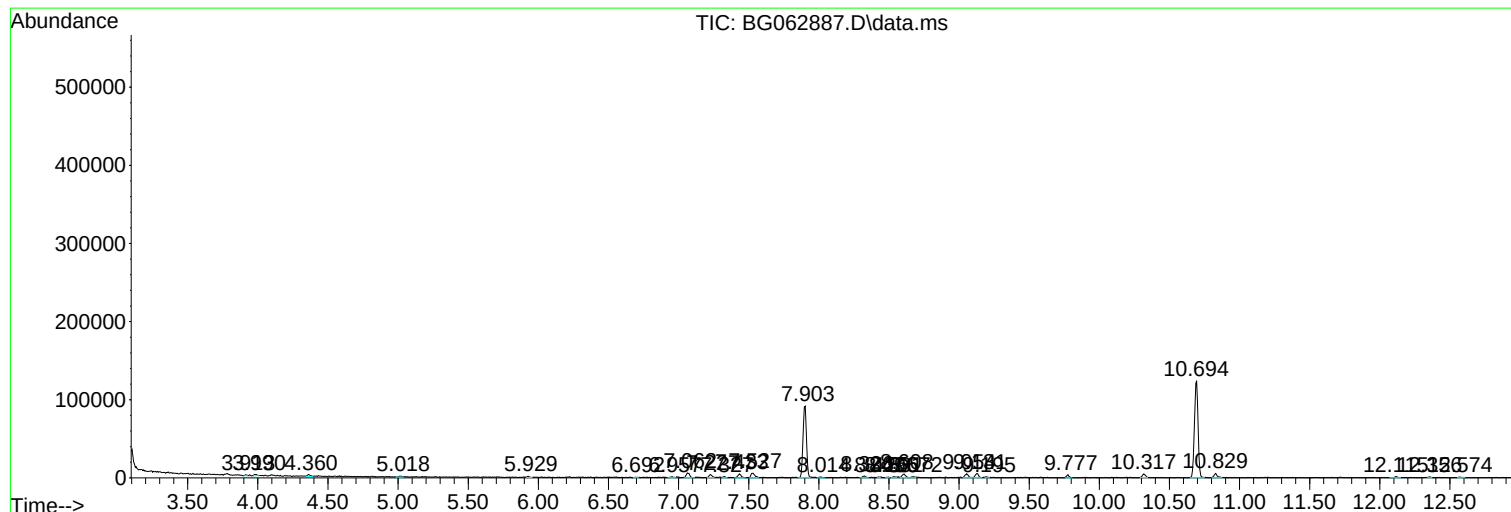

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062887.D
Acq On : 16 Sep 2024 20:10
Operator : JU/RC
Sample : P3899-11DL 20X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC12DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091324\
Data File : BG062887.D
Acq On : 16 Sep 2024 20:10
Operator : JU/RC
Sample : P3899-11DL 20X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC12DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc