


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091415\
 Data File : BG018660.D
 Acq On : 14 Sep 2015 13:54
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

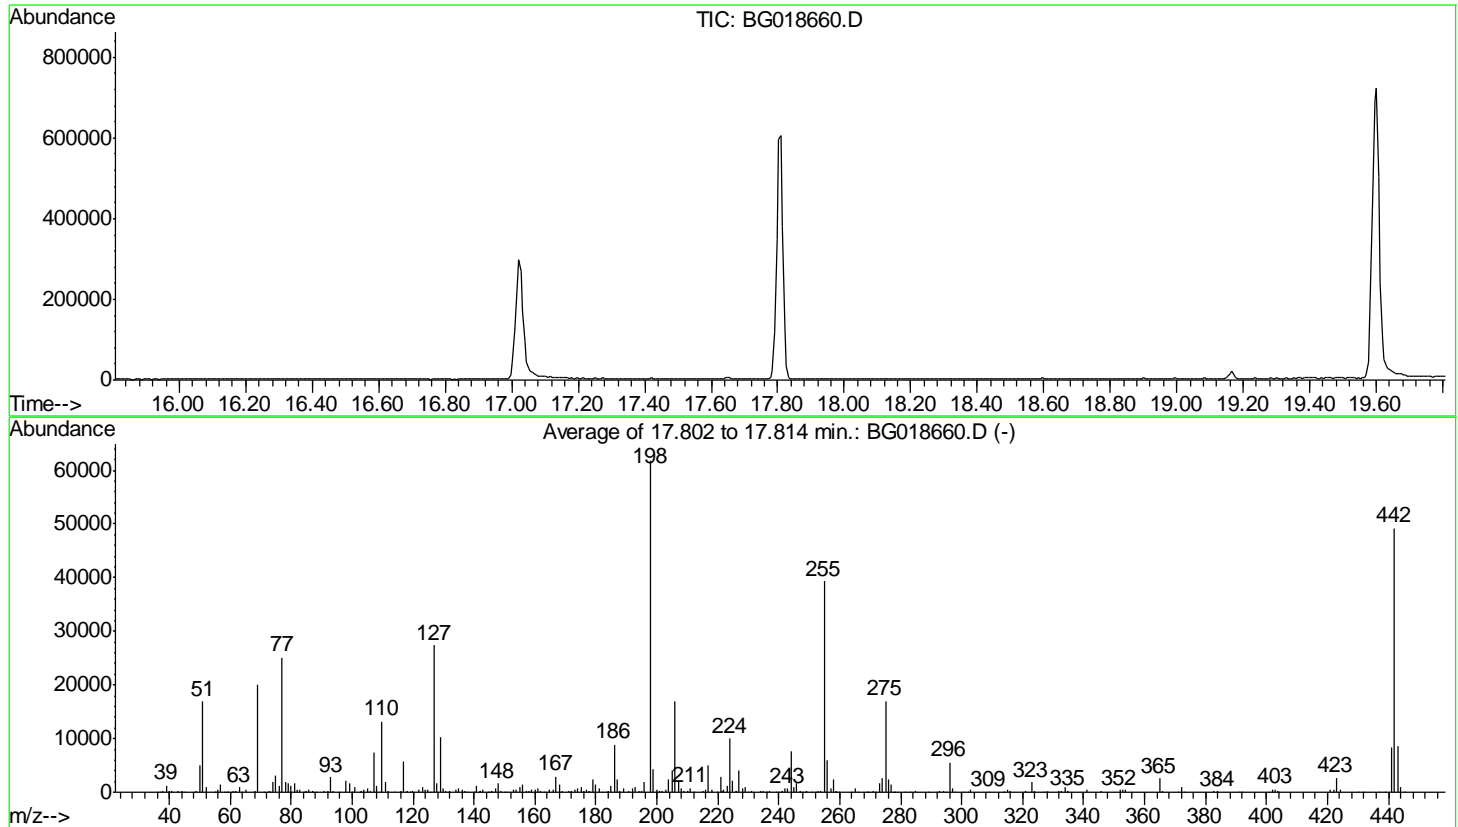

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	16859	PASS
68	69	0.00	2	1.6	316	PASS
69	198	0.00	100	32.5	20073	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	27360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61816	PASS
199	198	5	9	6.9	4250	PASS
275	198	10	60	27.4	16962	PASS
365	198	1	100	4.1	2514	PASS
441	442	0.01	24	16.9	8333	PASS
442	198	50	100	79.7	49266	PASS
443	442	15	24	17.6	8660	PASS