
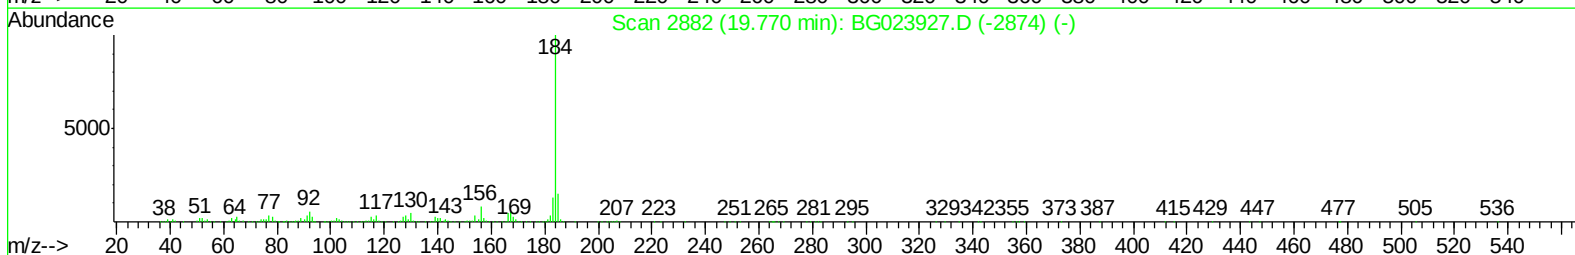
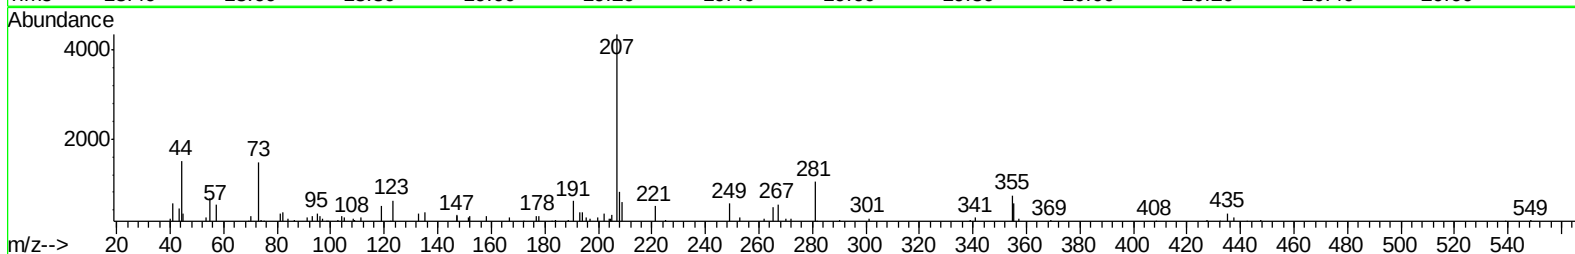


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091416\
 Data File : BG023982.D
 Acq On : 14 Sep 2016 13:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 00:59:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 09 16:24:09 2016
 Response via : Initial Calibration

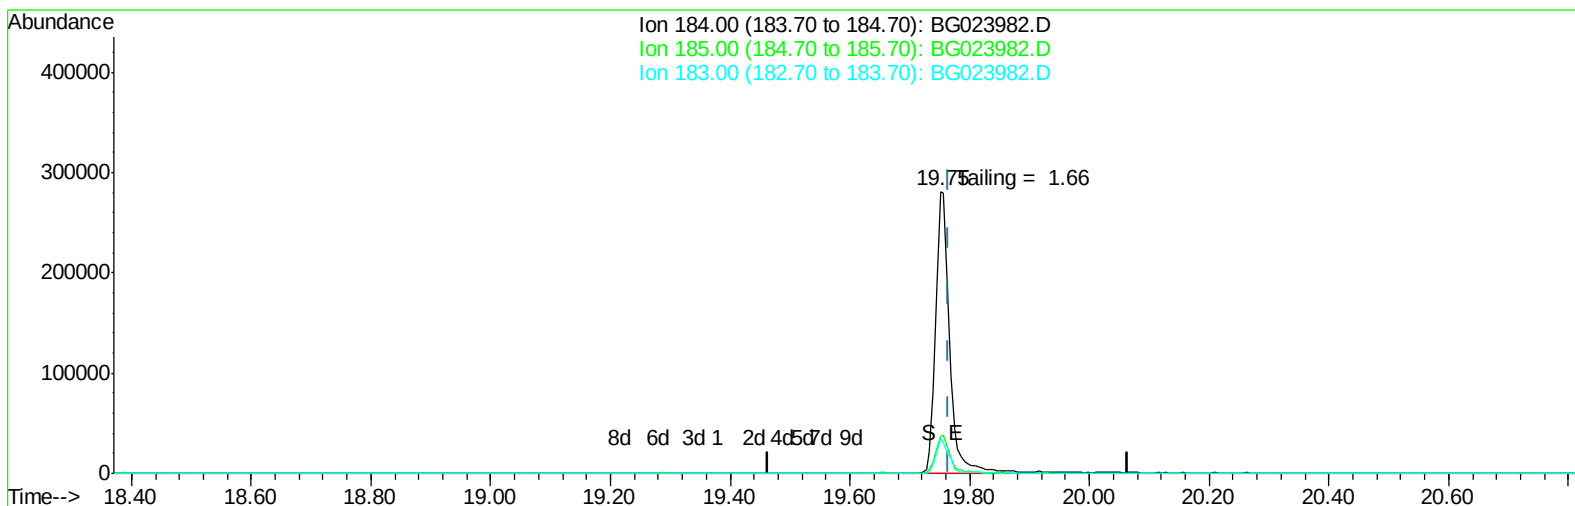

TIC: BG023982.D

(76) Benzidine




19.381min (-0.384) 13.13ng

response 63

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	13.40	90.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091416\
Data File : BG023982.D
Acq On : 14 Sep 2016 13:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 00:59:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 16:24:09 2016
Response via : Initial Calibration

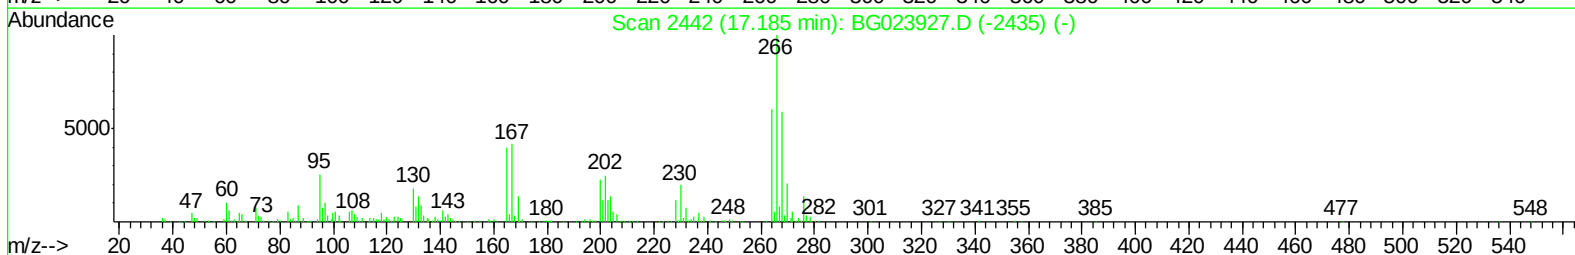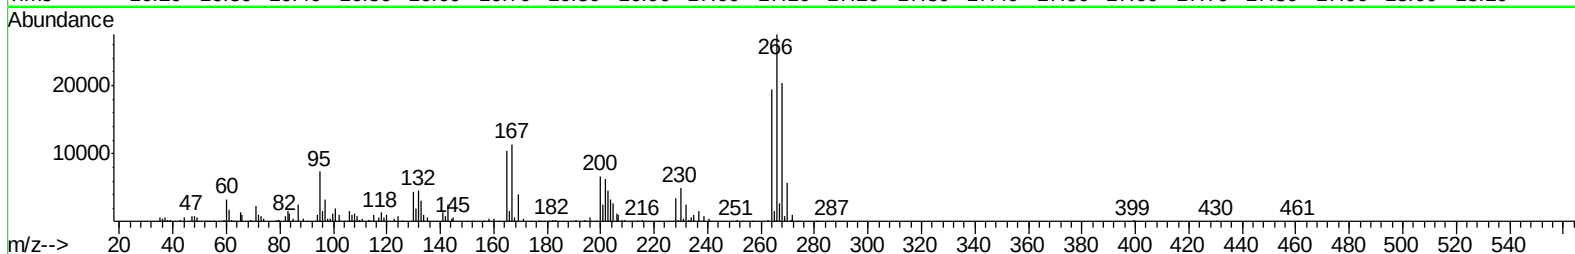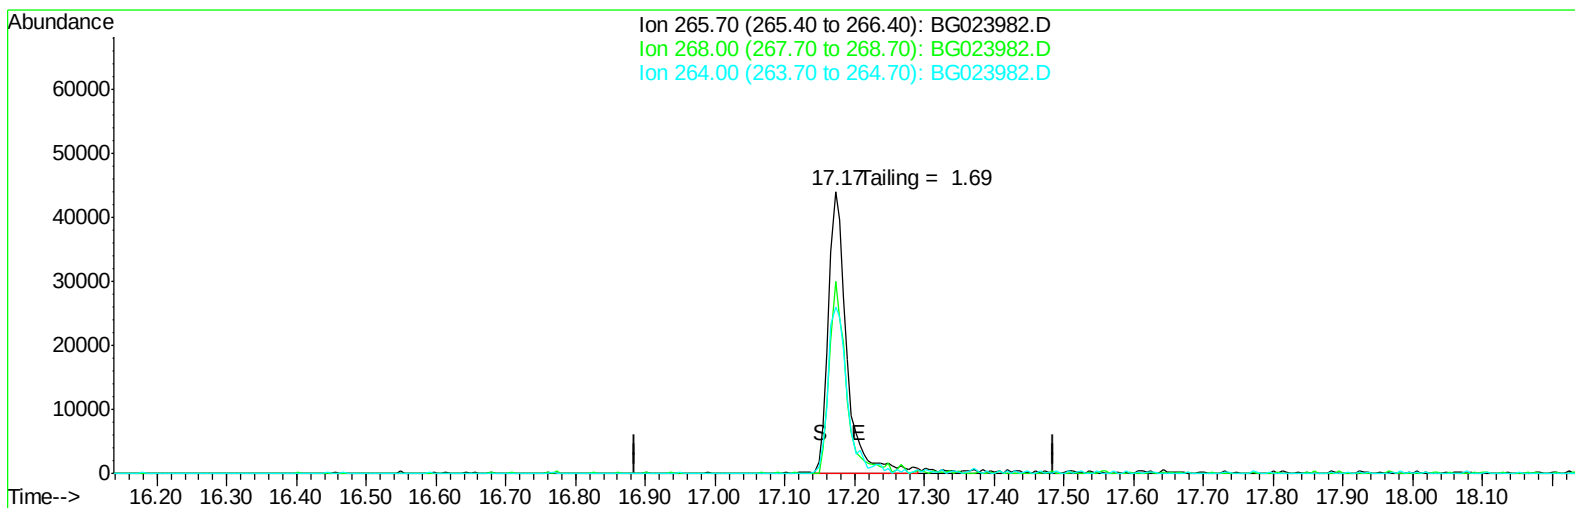

TIC: BG023982.D

(69) Pentachlorophenol (C)

17.186min (-17.186) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	64.90	0.00#
264.00	63.20	0.00#
0.00	0.00	0.00