


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091416\
 Data File : BG023982.D
 Acq On : 14 Sep 2016 13:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 09 16:24:09 2016

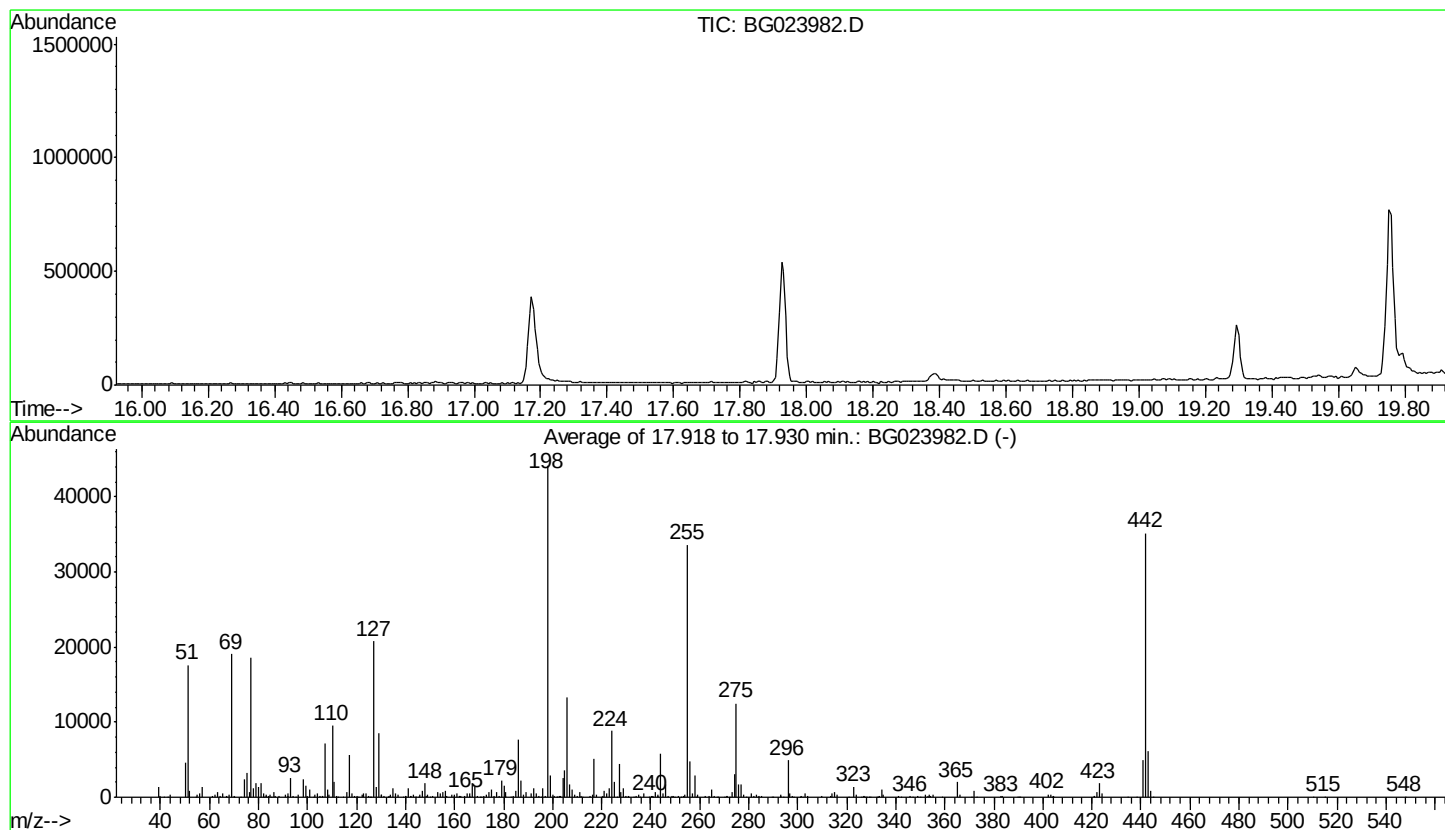

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	17621	PASS
68	69	0.00	2	1.7	329	PASS
69	198	0.00	100	43.2	19094	PASS
70	69	0.00	2	0.9	169	PASS
127	198	10	80	47.0	20757	PASS
197	198	0.00	2	0.5	218	PASS
198	198	100	100	100.0	44178	PASS
199	198	5	9	6.7	2958	PASS
275	198	10	60	28.2	12477	PASS
365	198	1	100	4.6	2017	PASS
441	442	0.01	24	14.3	5015	PASS
442	198	50	100	79.6	35178	PASS
443	442	15	24	17.3	6103	PASS