
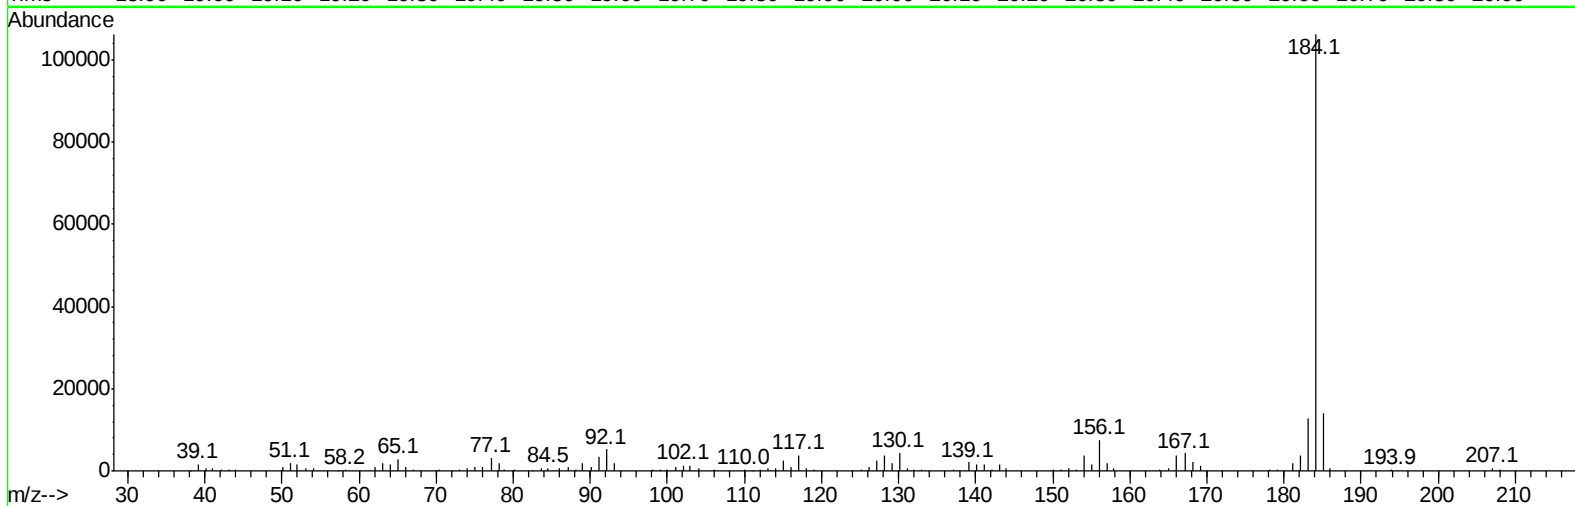


Data Path : Z:\HPCHEM1\BNA G\Data\BG091417\  
Data File : BG028728.D  
Acq On : 14 Sep 2017 12:06  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:13:35 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 16:57:11 2017  
Response via : Initial Calibration

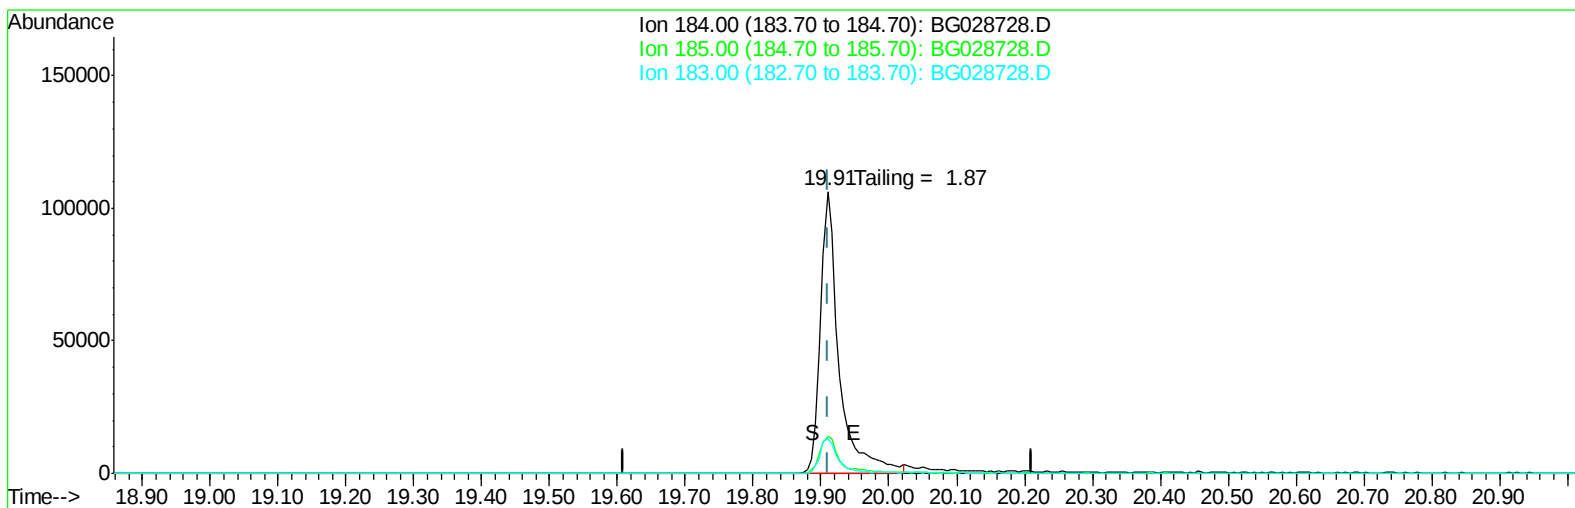

TIC: BG028728.D

(76) Benzidine



19.910min (-0.001) 0.00ng

response 198247

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 13.06 |
| 183.00 | 13.80 | 12.07 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\Data\BG091417\  
Data File : BG028728.D  
Acq On : 14 Sep 2017 12:06  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:13:35 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 16:57:11 2017  
Response via : Initial Calibration

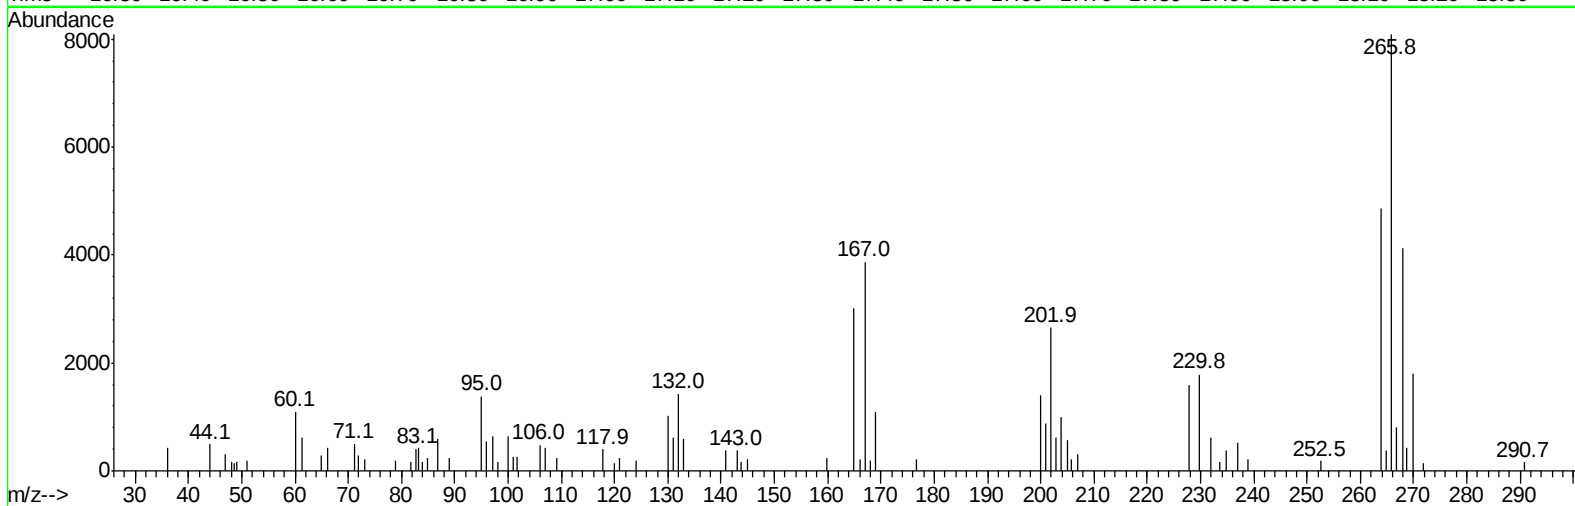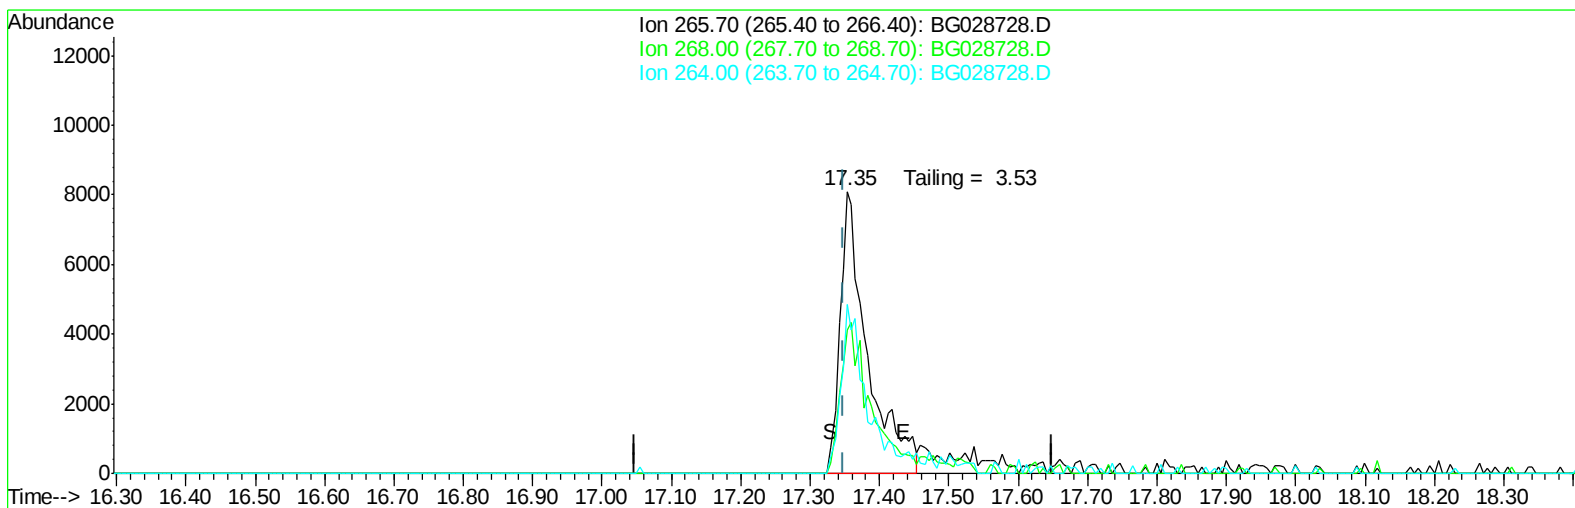

TIC: BG028728.D

(69) Pentachlorophenol (C)

17.354min (+0.005) 0.00ng m

response 22245

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 60.70 | 51.04 |
| 264.00 | 62.60 | 60.21 |
| 0.00   | 0.00  | 0.00  |