
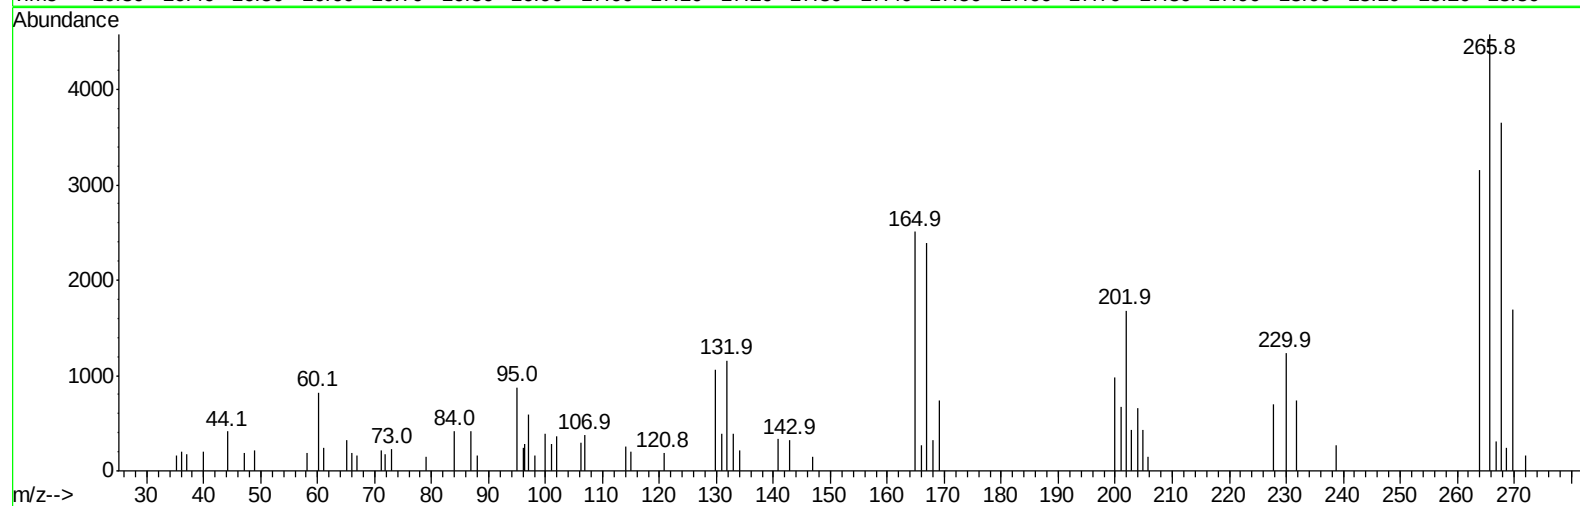


Data Path : Z:\HPCHEM1\BNA G\Data\BG091417\
Data File : BG028747.D
Acq On : 15 Sep 2017 00:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:16:49 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

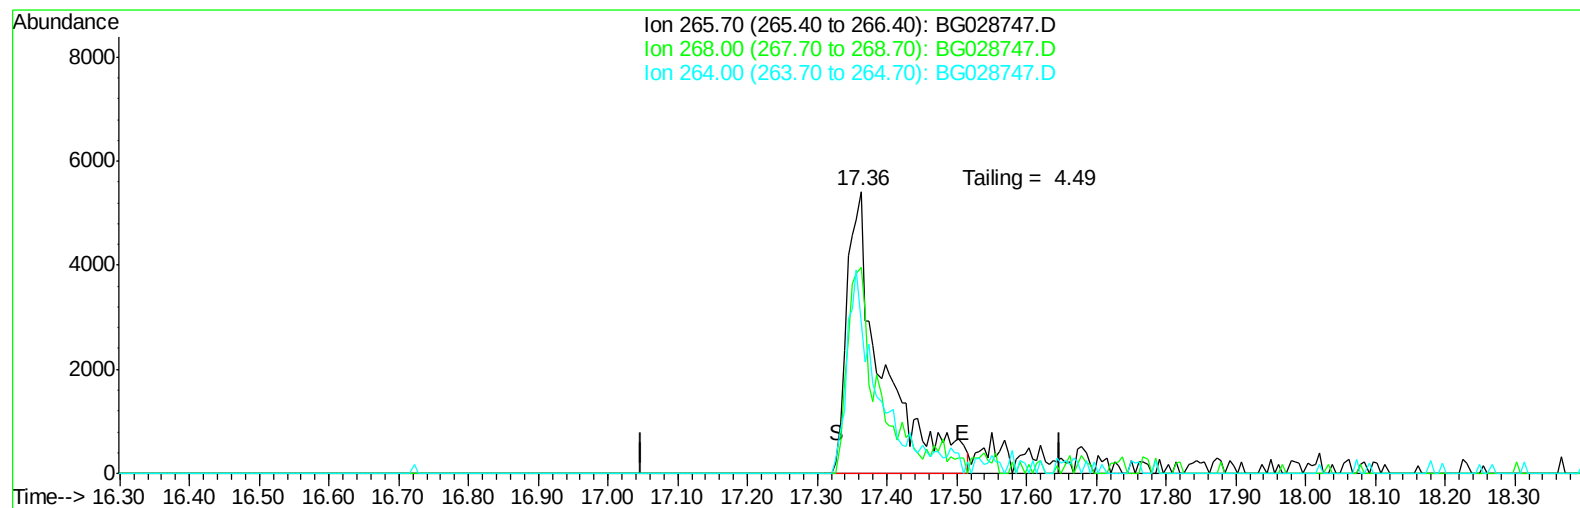

TIC: BG028747.D

(69) Pentachlorophenol (C)



17.349min (-17.349) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG091417\
Data File : BG028747.D
Acq On : 15 Sep 2017 00:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:16:49 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

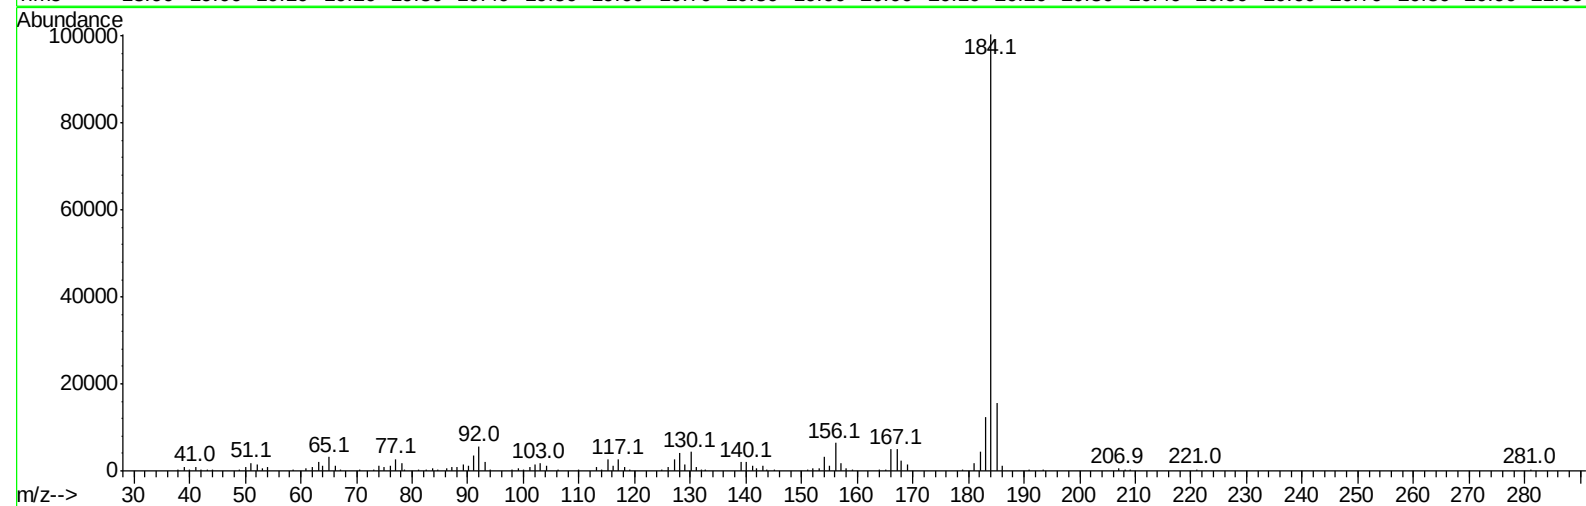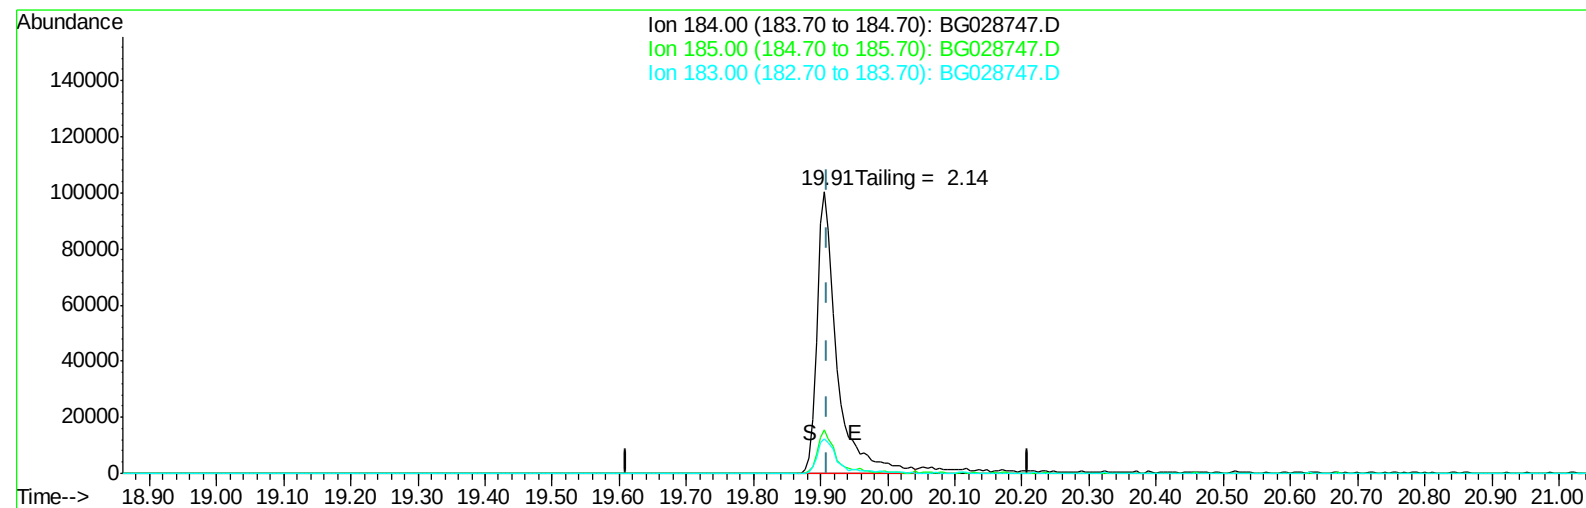

TIC: BG028747.D

(76) Benzidine

19.906min (-0.004) 0.00ng

response 203192

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.49
183.00	13.80	12.40
0.00	0.00	0.00