

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
 Data File : BG028737.D
 Acq On : 14 Sep 2017 18:01
 Operator : SJ/JU
 Sample : I5187-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20170607-COMP-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.436	308	314	324	rVB	35221	57510	2.41%	0.580%
2	5.900	387	393	408	rBV	323763	557700	23.36%	5.622%
3	7.481	655	662	675	rBV	320242	619037	25.93%	6.241%
4	7.862	720	727	737	rBV	313798	567302	23.76%	5.719%
5	8.327	799	806	816	rVB3	65963	118802	4.98%	1.198%
6	8.656	852	862	873	rVB	220839	399472	16.73%	4.027%
7	9.496	997	1005	1017	rBV	184265	361536	15.14%	3.645%
8	11.147	1280	1286	1296	rBV2	83094	163142	6.83%	1.645%
9	13.562	1688	1697	1709	rBV	571991	931325	39.01%	9.389%
10	14.378	1831	1836	1846	rBV	53911	95044	3.98%	0.958%
11	14.942	1924	1932	1941	rBV2	178816	314599	13.18%	3.172%
12	16.429	2178	2185	2202	rBV	780308	1301171	54.50%	13.118%
13	17.692	2393	2400	2411	rVB2	356667	578397	24.23%	5.831%
14	18.550	2541	2546	2549	rBV3	16914	32447	1.36%	0.327%
15	20.277	2833	2840	2848	rBV	1780378	2387477	100.00%	24.069%
16	21.593	3058	3064	3068	rBV8	12982	25454	1.07%	0.257%
17	22.022	3130	3137	3147	rVB2	385640	707765	29.64%	7.135%
18	25.518	3719	3732	3748	rBV2	209060	701094	29.37%	7.068%


Sum of corrected areas: 9919274

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028737.D
Acq On : 14 Sep 2017 18:01
Operator : SJ/JU
Sample : I5187-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20170607-COMP-D

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

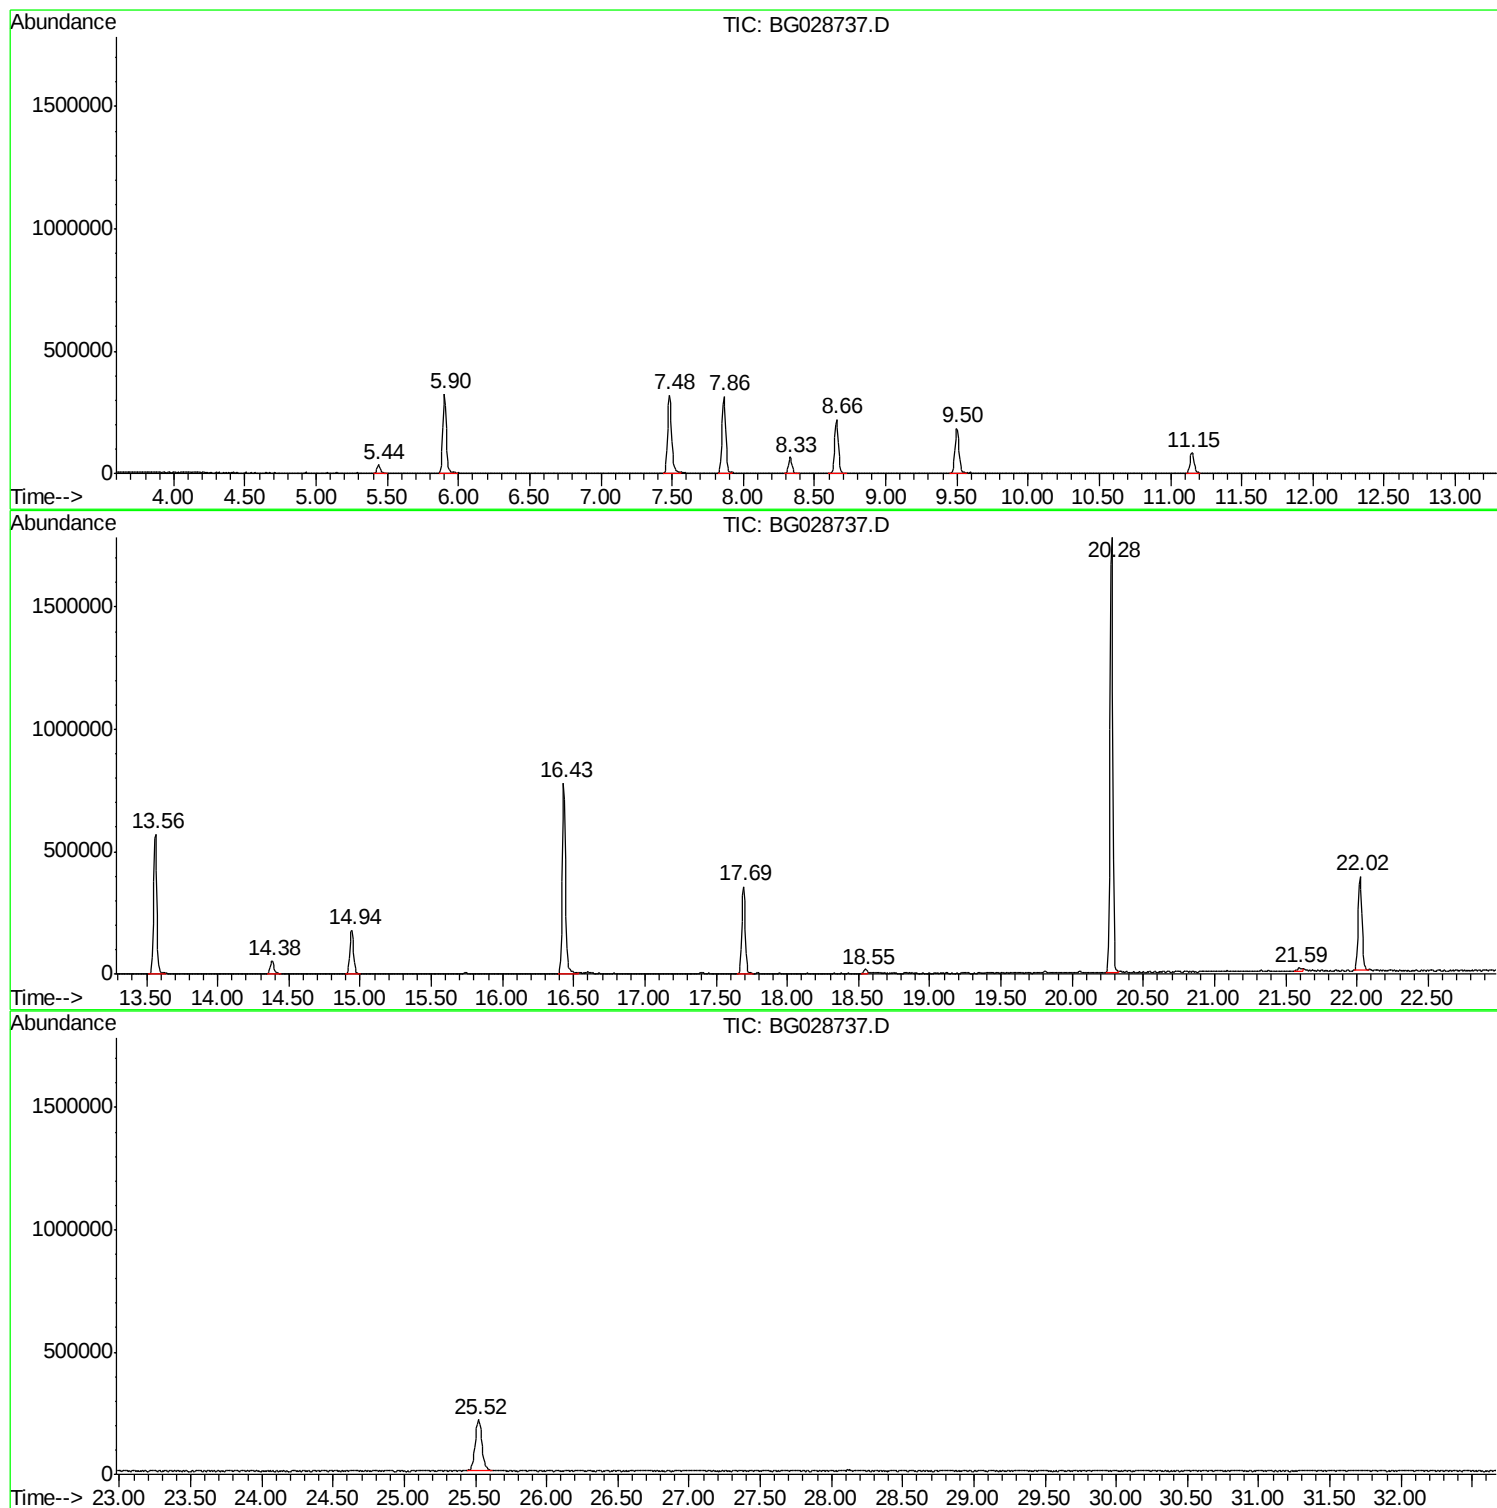

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028737.D
Acq On : 14 Sep 2017 18:01
Operator : SJ/JU
Sample : I5187-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20170607-COMP-D










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.44 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.44	9.68 ng	57510	1,4-Dichlorobenzene-d4	8.33

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	47
2			2,2,3,3,5,8,11-Heptamethyl-4,7,1...	348	C18H40O4Si	1000367-07-2	28
3			Hvdrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	28
4			3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	27
5			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	25

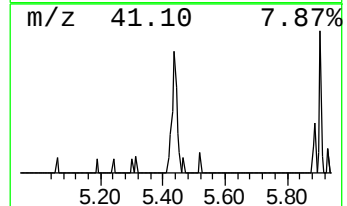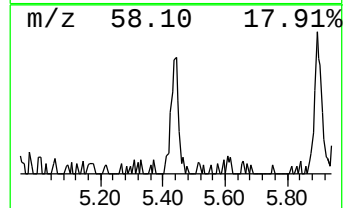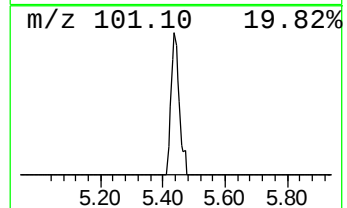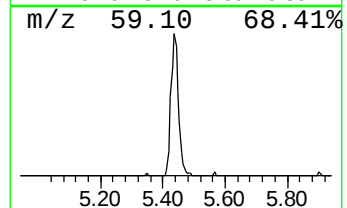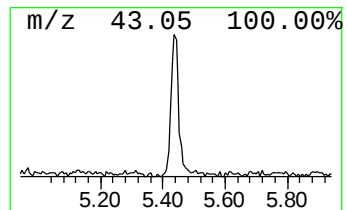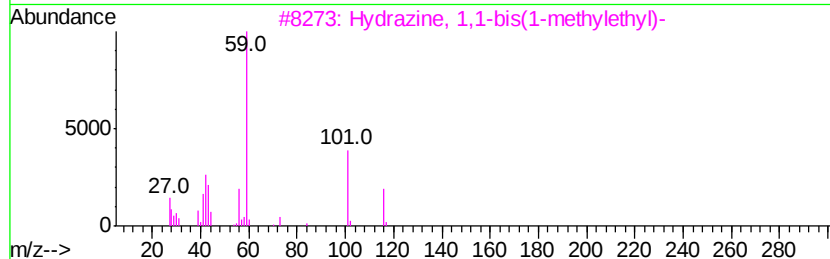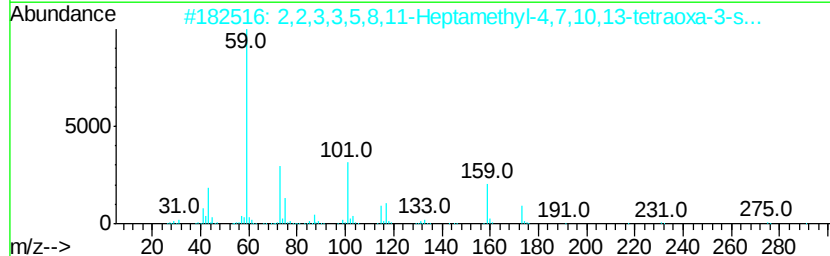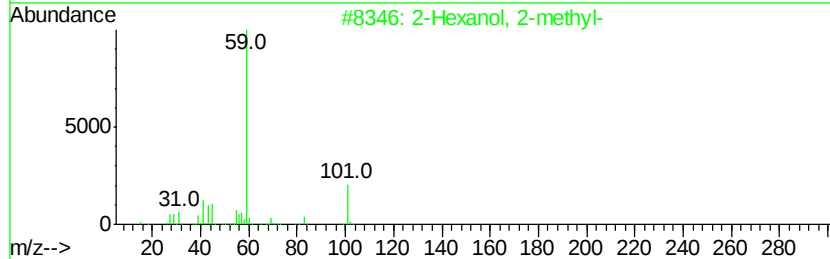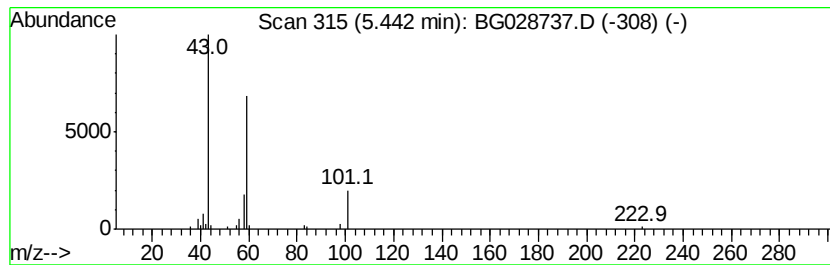

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028737.D
Acq On : 14 Sep 2017 18:01
Operator : SJ/JU
Sample : I5187-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20170607-COMP-D










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.86 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.86	95.50 ng	567302	1,4-Dichlorobenzene-d4	8.33

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	14
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	13

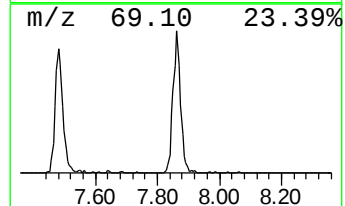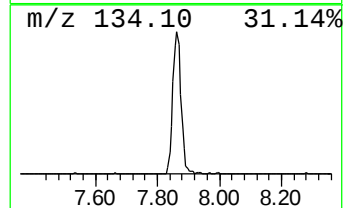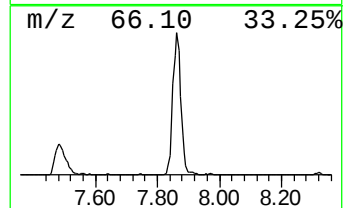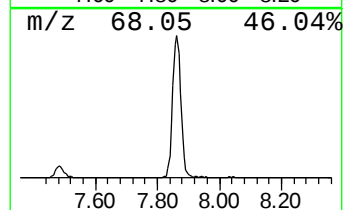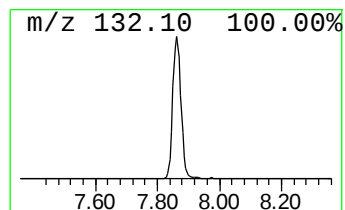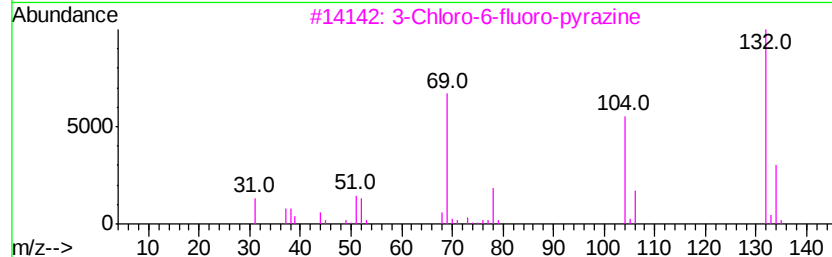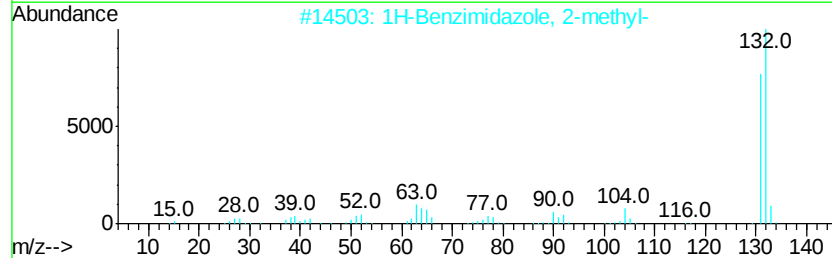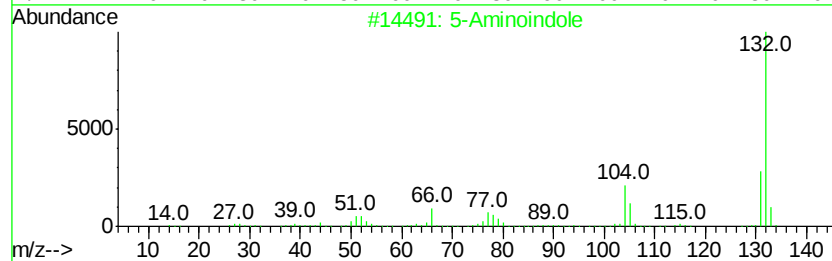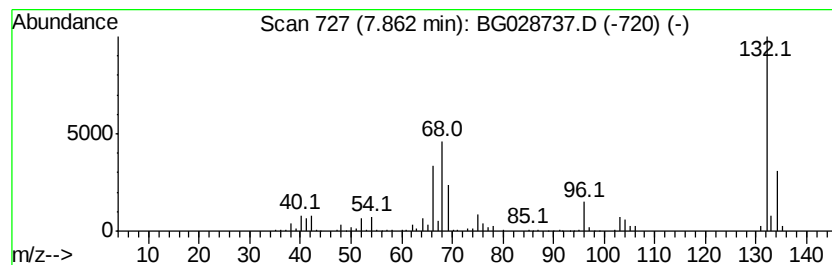

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG091417\
Data File : BG028737.D
Acq On : 14 Sep 2017 18:01
Operator : SJ/JU
Sample : I5187-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20170607-COMP-D

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.44	5.44	9.7	ng	57510	1	8.33	118802	20.0
unknown7.86	7.86	95.5	ng	567302	1	8.33	118802	20.0