

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
 Data File : BG028760.D
 Acq On : 15 Sep 2017 9:16
 Operator : SJ/JU
 Sample : I5223-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 090917-SIDI-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.439	308	315	322	rBV	53409	91800	2.92%	0.799%
2	5.897	386	393	407	rBV	246881	431856	13.76%	3.760%
3	7.478	654	662	676	rBV	196066	388863	12.39%	3.386%
4	7.859	720	727	737	rBV	315035	566350	18.04%	4.931%
5	8.324	800	806	814	rBV	102848	184194	5.87%	1.604%
6	8.653	853	862	873	rBV	392090	696893	22.20%	6.068%
7	9.499	998	1006	1020	rBV	312319	594777	18.95%	5.179%
8	11.144	1278	1286	1299	rBV	129388	259814	8.28%	2.262%
9	13.559	1688	1697	1709	rBV	1041212	1606904	51.19%	13.991%
10	14.939	1925	1932	1944	rBV3	232552	421868	13.44%	3.673%
11	16.426	2179	2185	2200	rBV	605951	1020578	32.51%	8.886%
12	17.689	2391	2400	2409	rBV	398730	634537	20.21%	5.525%
13	19.934	2776	2782	2787	rBV3	29685	37546	1.20%	0.327%
14	20.274	2834	2840	2847	rBV	2408818	3139073	100.00%	27.332%
15	22.019	3129	3137	3146	rBV	396892	741541	23.62%	6.457%
16	25.515	3722	3732	3745	rBV2	210292	668286	21.29%	5.819%


Sum of corrected areas: 11484880

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028760.D
Acq On : 15 Sep 2017 9:16
Operator : SJ/JU
Sample : I5223-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
090917-SIDI-E-D-S

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

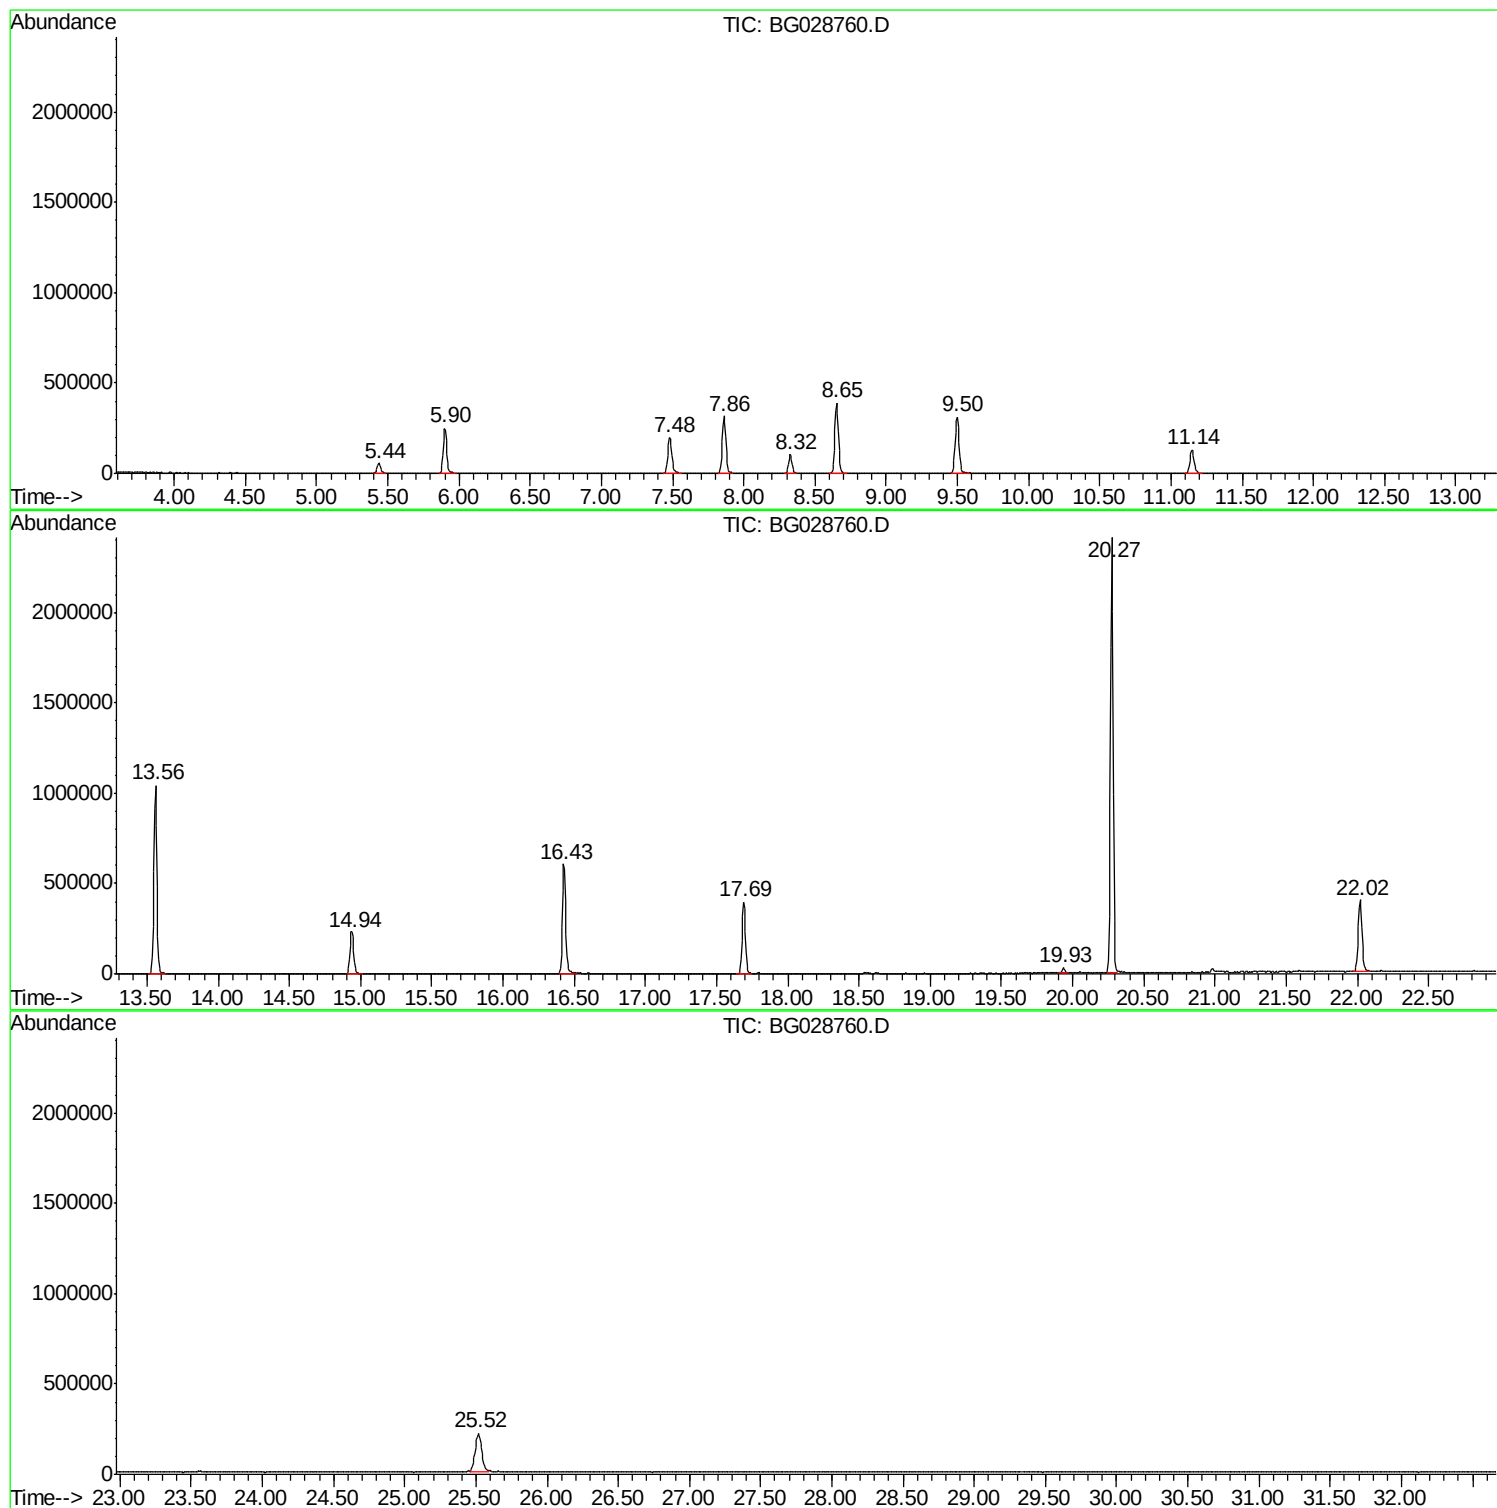

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028760.D
Acq On : 15 Sep 2017 9:16
Operator : SJ/JU
Sample : I5223-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
090917-SIDI-E-D-S










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.44 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.44	9.97 ng	91800	1,4-Dichlorobenzene-d4	8.32

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42		
2	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36		
3	3-Hexanol	102	C6H14O	000623-37-0	28		
4	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23		
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		

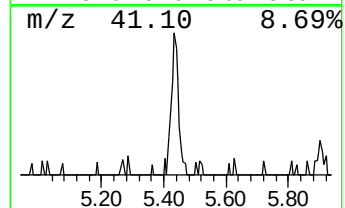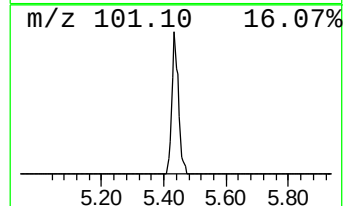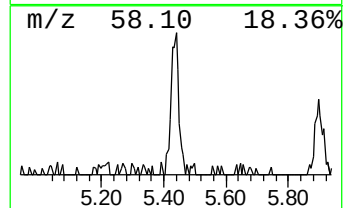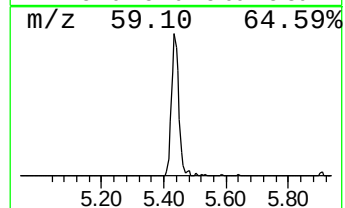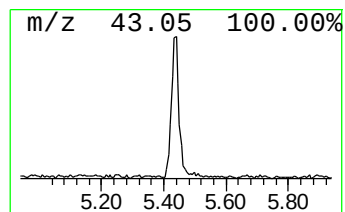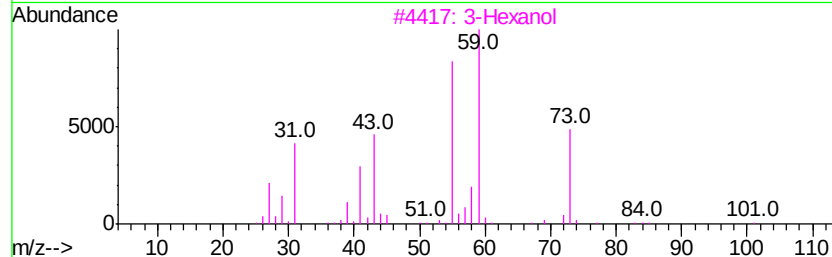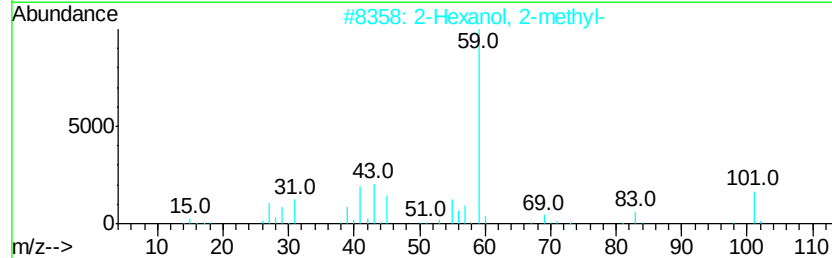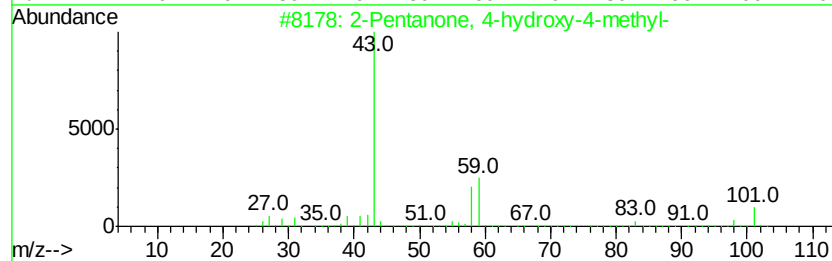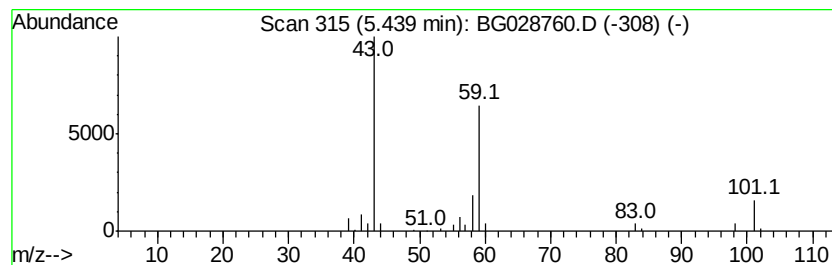

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG091417\
Data File : BG028760.D
Acq On : 15 Sep 2017 9:16
Operator : SJ/JU
Sample : I5223-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
090917-SIDI-E-D-S










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.86 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.86	61.49 ng	566350	1,4-Dichlorobenzene-d4	8.32

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	16
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

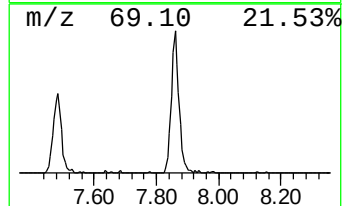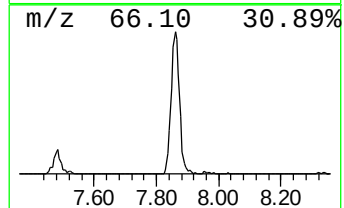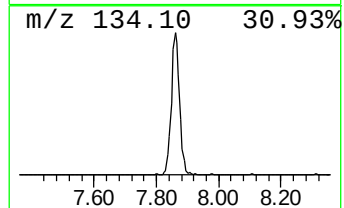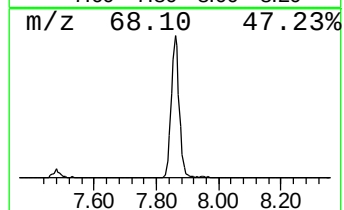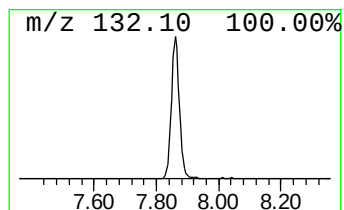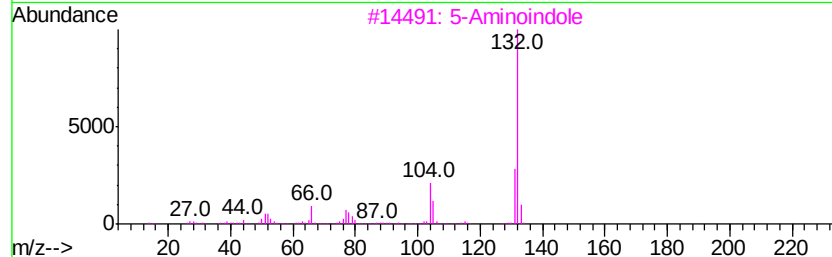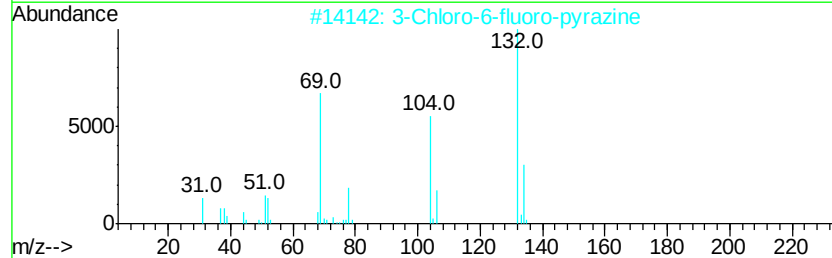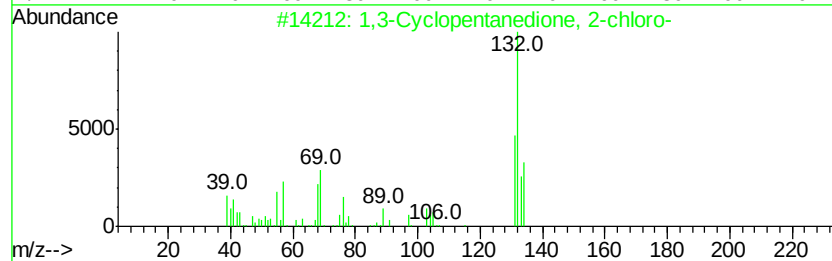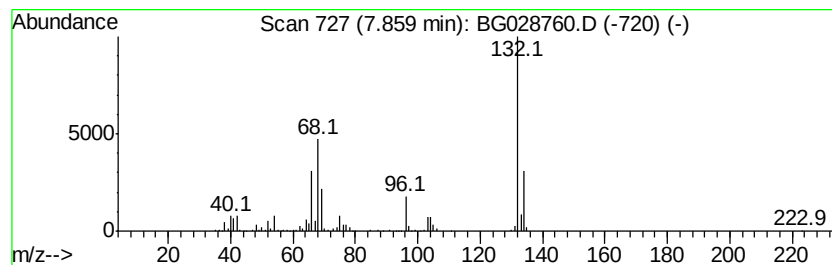

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG091417\
Data File : BG028760.D
Acq On : 15 Sep 2017 9:16
Operator : SJ/JU
Sample : I5223-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
090917-SIDI-E-D-S

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.44	5.44	10.0	ng	91800	1	8.32	184194	20.0
unknown7.86	7.86	61.5	ng	566350	1	8.32	184194	20.0