


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG091417\  
 Data File : BG028728.D  
 Acq On : 14 Sep 2017 12:06  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG091217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 12 16:57:11 2017

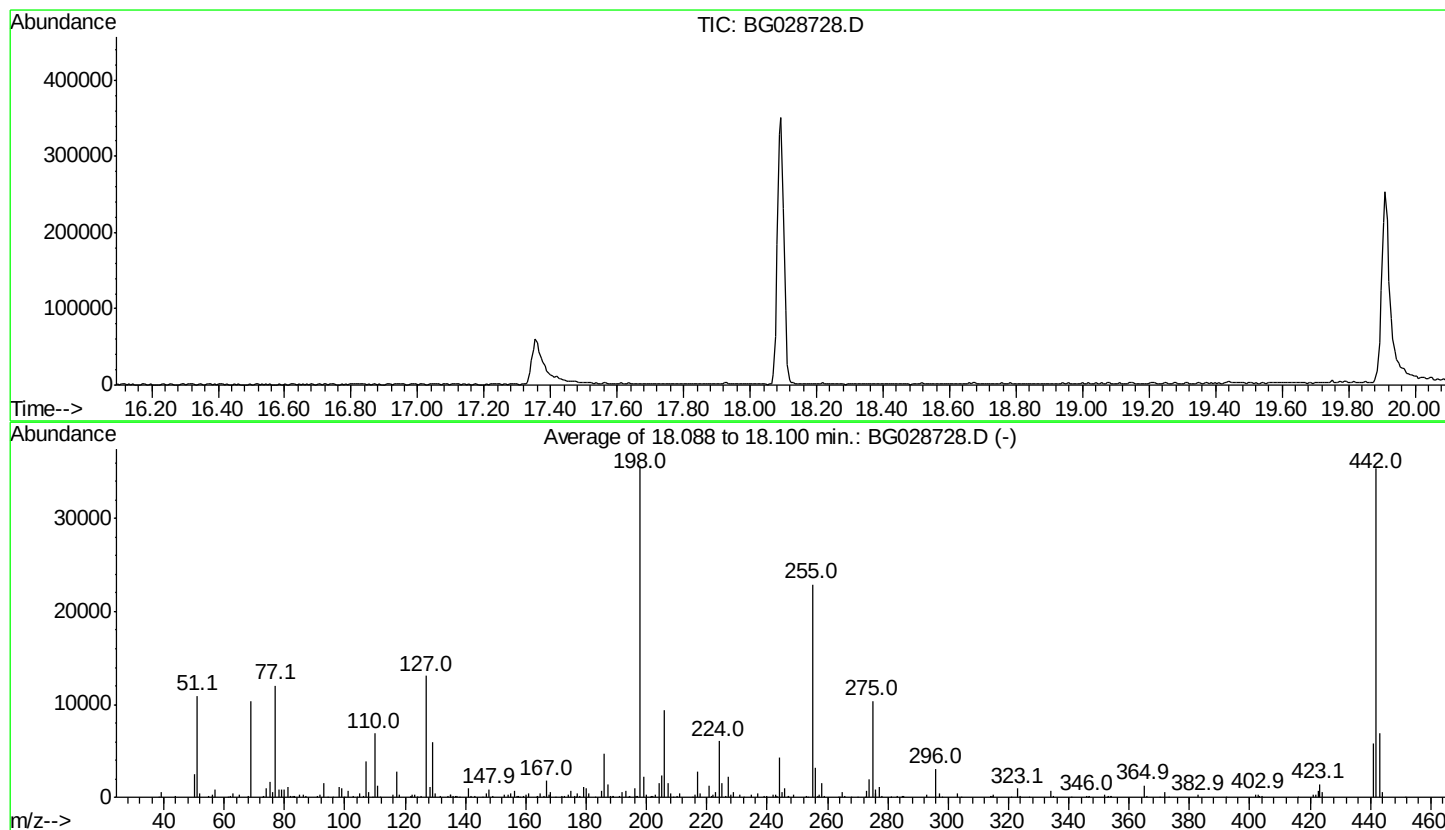

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 30.6      | 10918   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 167     | PASS             |
| 69          | 198          | 0.00         | 100          | 29.0      | 10355   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 36.6      | 13065   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 86      | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 35720   | PASS             |
| 199         | 198          | 5            | 9            | 6.2       | 2222    | PASS             |
| 275         | 198          | 10           | 60           | 29.1      | 10411   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 1272    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.2      | 5743    | PASS             |
| 442         | 198          | 50           | 100          | 99.4      | 35498   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 6951    | PASS             |