


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG091417\
 Data File : BG028747.D
 Acq On : 15 Sep 2017 00:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

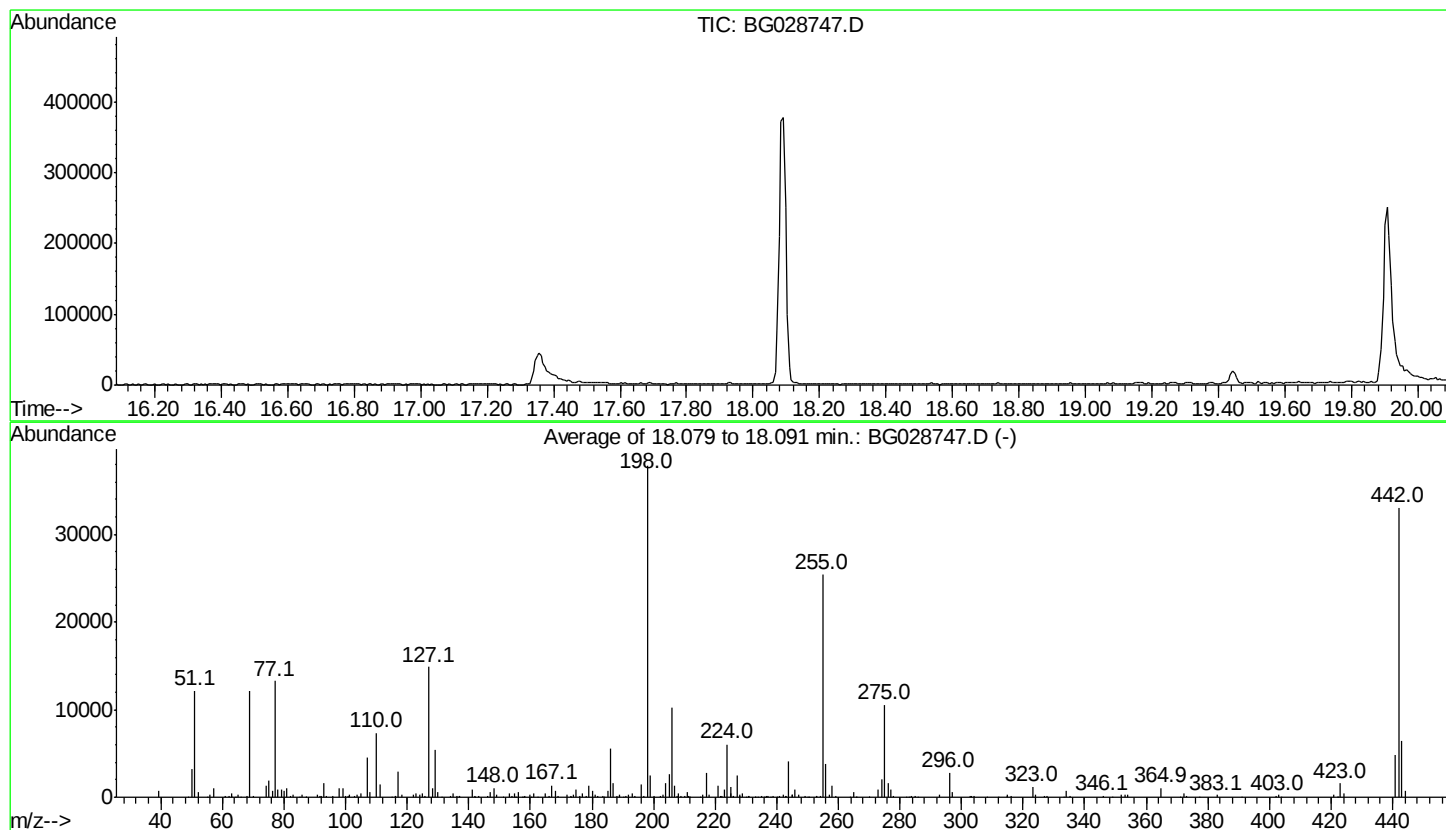

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	12190	PASS
68	69	0.00	2	0.9	104	PASS
69	198	0.00	100	31.9	12085	PASS
70	69	0.00	2	0.6	78	PASS
127	198	10	80	39.2	14851	PASS
197	198	0.00	2	0.3	126	PASS
198	198	100	100	100.0	37864	PASS
199	198	5	9	6.4	2440	PASS
275	198	10	60	27.8	10529	PASS
365	198	1	100	2.9	1096	PASS
441	442	0.01	24	14.5	4802	PASS
442	198	50	100	87.4	33096	PASS
443	442	15	24	19.5	6469	PASS