

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091420\
 Data File : BG046604.D
 Acq On : 14 Sep 2020 15:30
 Operator : CG/JU
 Sample : PB131580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB131580BL

Quant Time: Sep 14 17:27:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	60421	20.00	ng	0.00
21) Naphthalene-d8	10.72	136	240131	20.00	ng	0.00
39) Acenaphthene-d10	14.55	164	171342	20.00	ng	0.00
64) Phenanthrene-d10	17.30	188	452197	20.00	ng	0.00
76) Chrysene-d12	21.55	240	504588	20.00	ng	0.00
86) Perylene-d12	24.65	264	475717	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	393309	115.29	ng	0.00
7) Phenol-d6	7.10	99	510093	105.48	ng	0.00
23) Nitrobenzene-d5	9.08	82	332744	79.20	ng	0.00
42) 2,4,6-Tribromophenol	16.05	330	246186	106.04	ng	0.00
45) 2-Fluorobiphenyl	13.18	172	929167	82.78	ng	0.00
79) Terphenyl-d14	19.91	244	1695322	71.50	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.08	70	41695	14.414	ng	# 74
51) 2,6-Dinitrotoluene	14.55	165	21952	7.513	ng	# 32
57) 2,4-Dinitrotoluene	14.55	165	21952	5.269	ng	# 32
67) 4-Bromophenyl-phenylether	16.05	248	18318	3.472	ng	# 1
77) Benzidine	19.91	184	25529	2.177	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091420\
Data File : BG046604.D
Acq On : 14 Sep 2020 15:30
Operator : CG/JU
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB131580BL

Quant Time: Sep 14 17:27:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

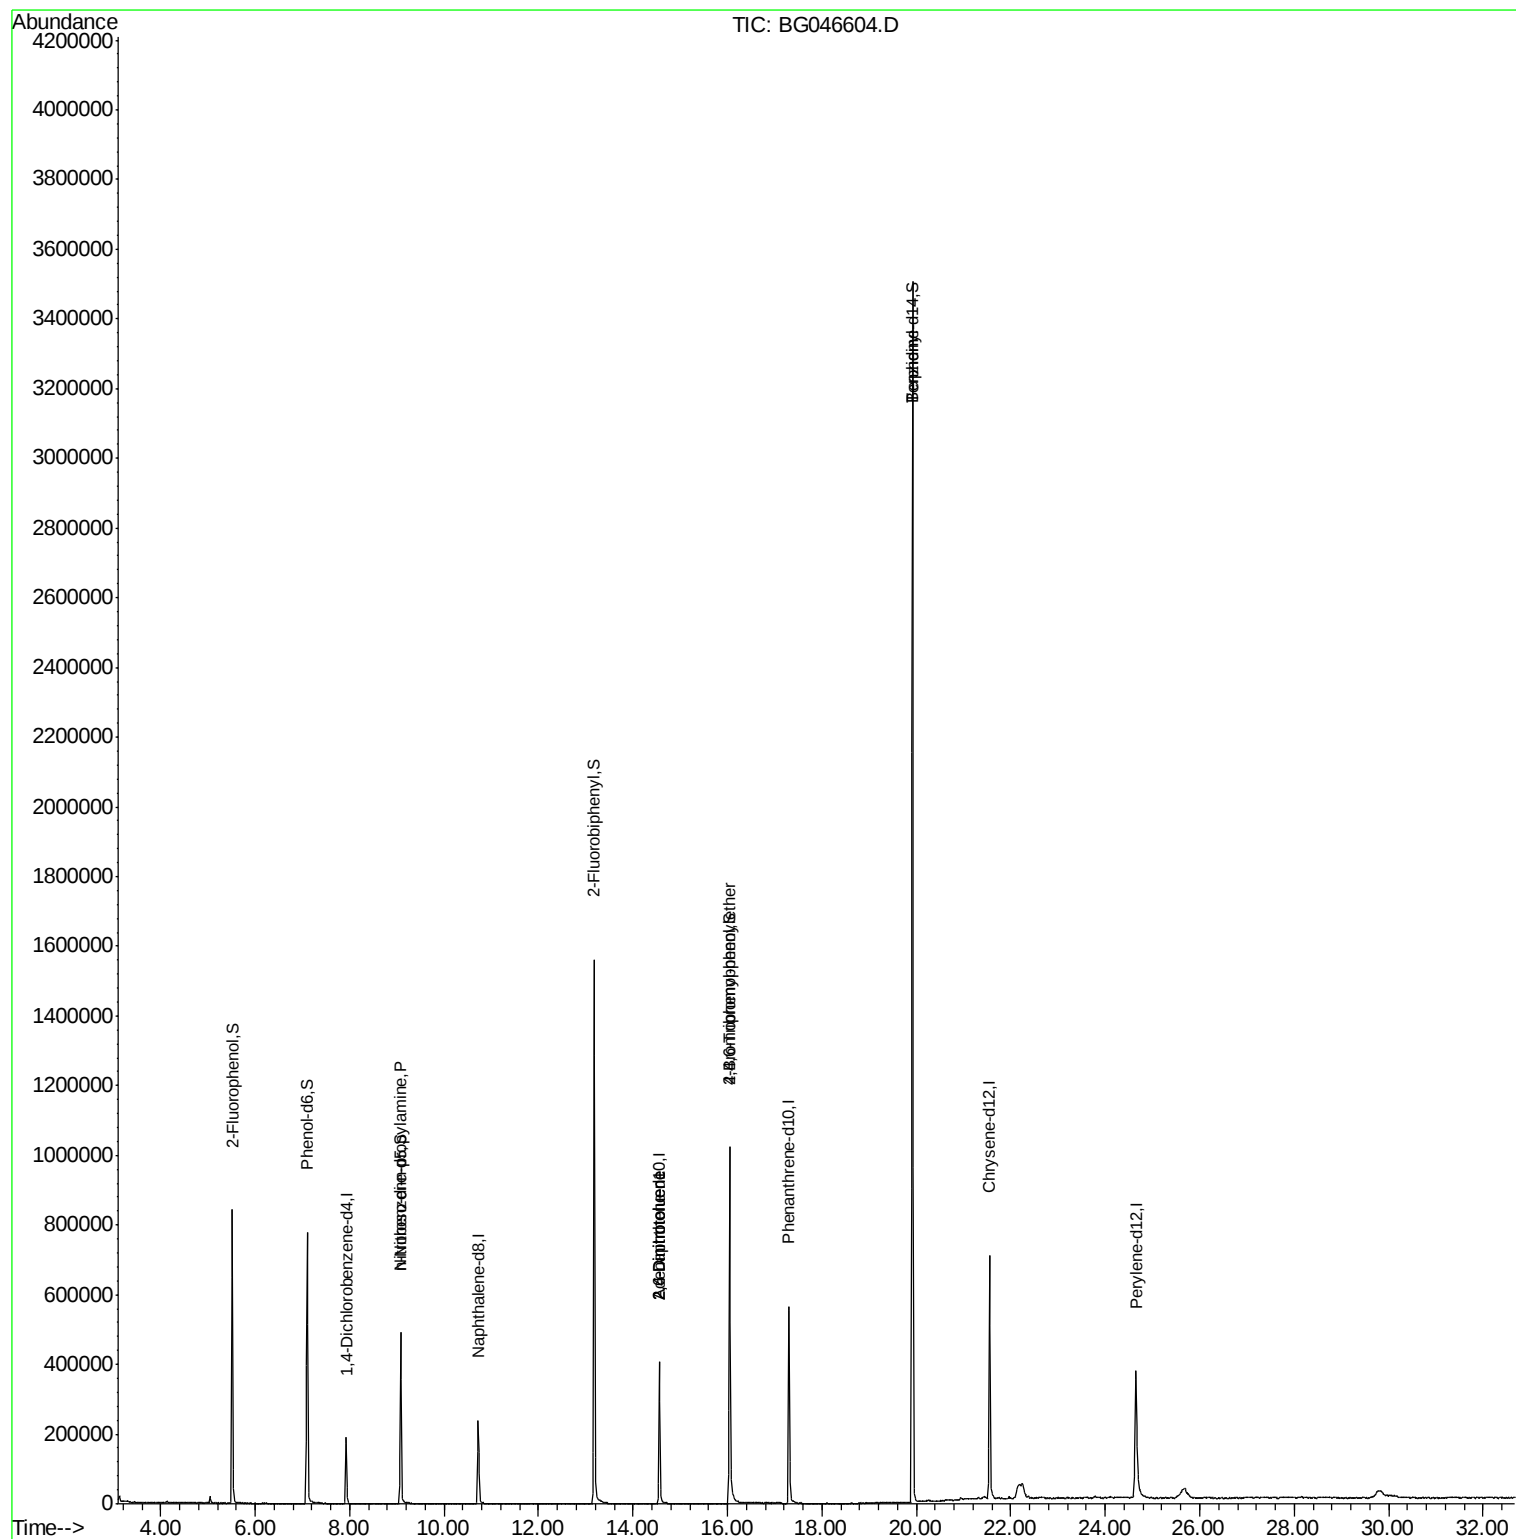

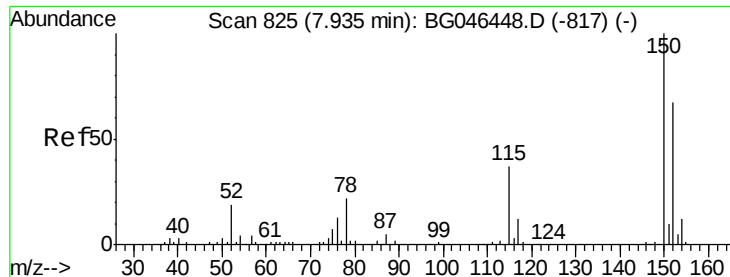


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.93 min Scan# 823
Delta R.T. -0.01 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Instrument :
BNA_G
ClientSampleId :
PB131580BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	142.9	119.5	179.3
115	50.3	44.3	66.5

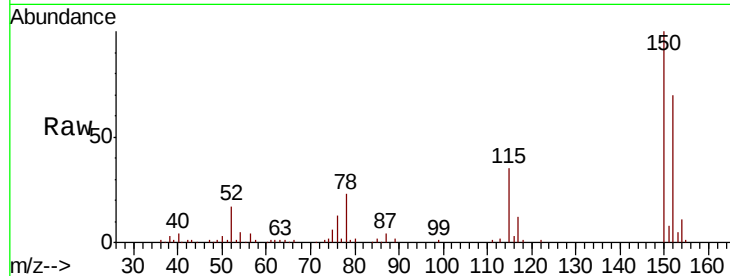


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

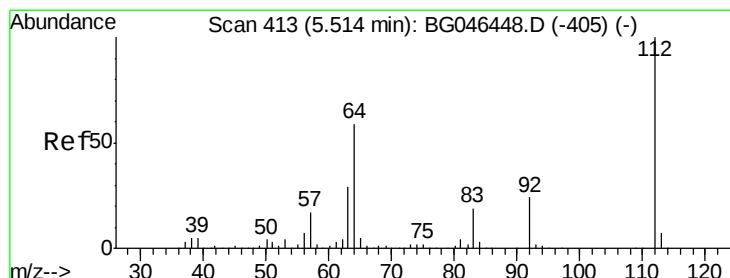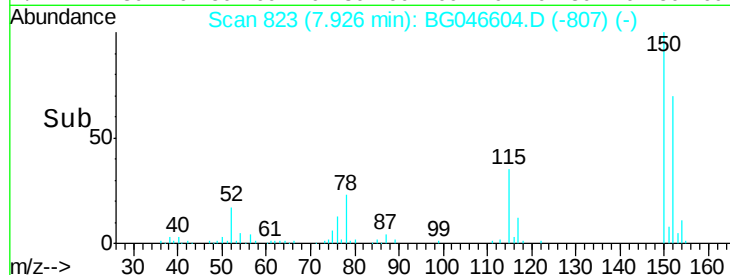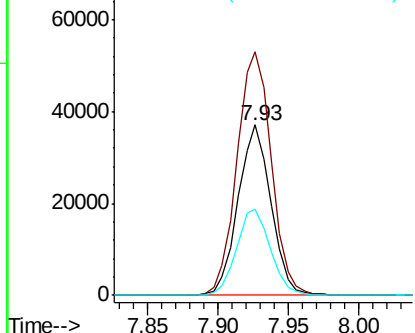



#5


2-Fluorophenol
Concen: 115.295 ng
RT: 5.51 min Scan# 412
Delta R.T. -0.00 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.7	47.0	70.6
63	30.0	23.5	35.3

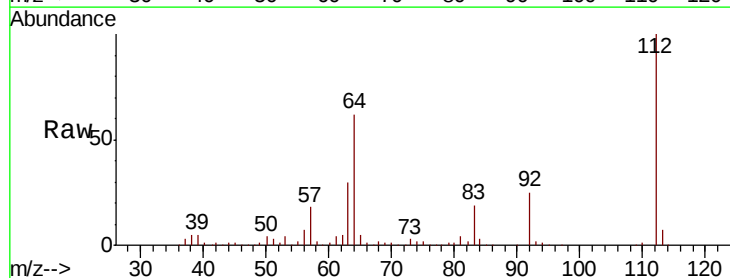

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

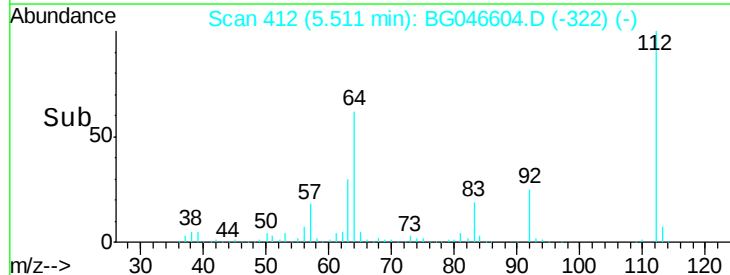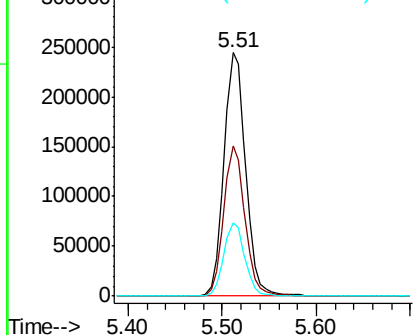

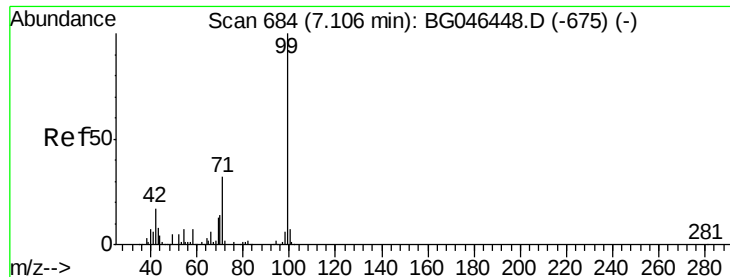

#7

Phenol-d6

Concen: 105.480 ng

RT: 7.10 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30

Instrument :

BNA_G

ClientSampleId :

PB131580BL


Tot Ion: 99 Resp: 510093

Ion Ratio Lower Upper




99 100

42 16.2 13.3 19.9

71 31.4 25.3 37.9

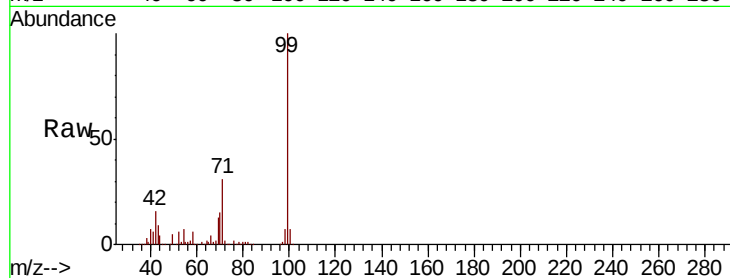

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

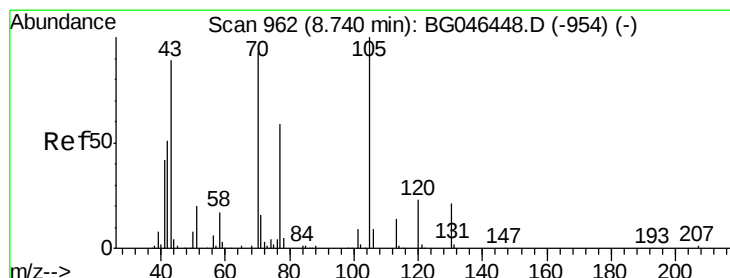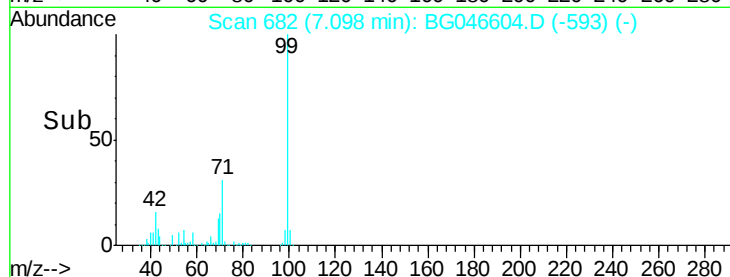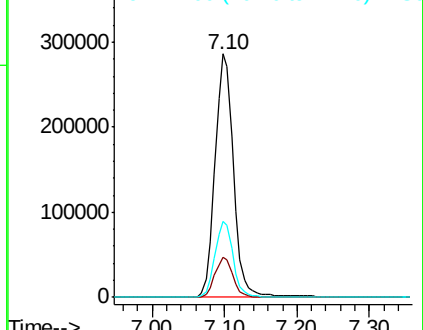

#19

n-Nitroso-di-n-propylamine

Concen: 14.414 ng

RT: 9.08 min Scan# 1019

Delta R.T. 0.34 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30

Tgt Ion: 70 Resp: 41695


Ion Ratio Lower Upper

70 100



42 41.6 44.2 66.2#

101 0.0 7.8 11.8#

130 1.7 18.2 27.4#

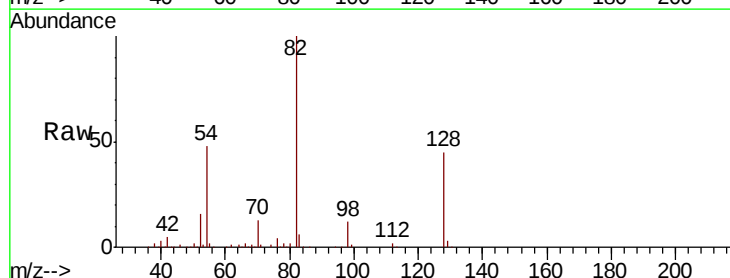

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

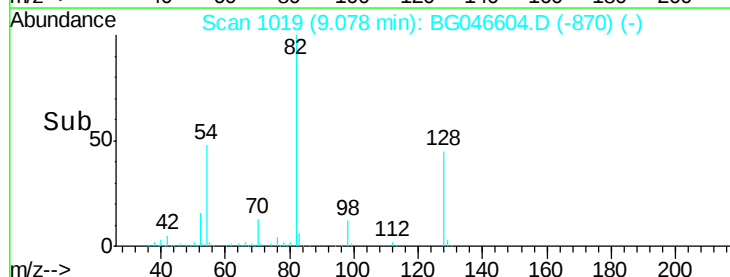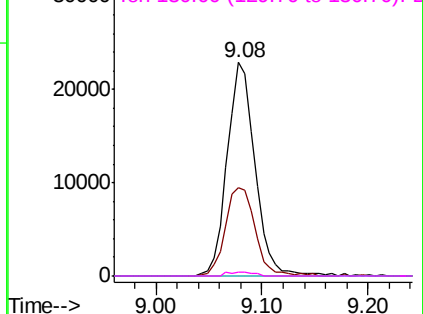







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.72 min Scan# 1299
Delta R.T. -0.00 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Instrument :
BNA_G
ClientSampleId :
PB131580BL

Tot Ion:136	Resp:	240131
Ion	Ratio	Lower Upper
136	100	
137	11.3	8.8 13.2
54	8.0	6.1 9.1
68	5.9	4.8 7.2

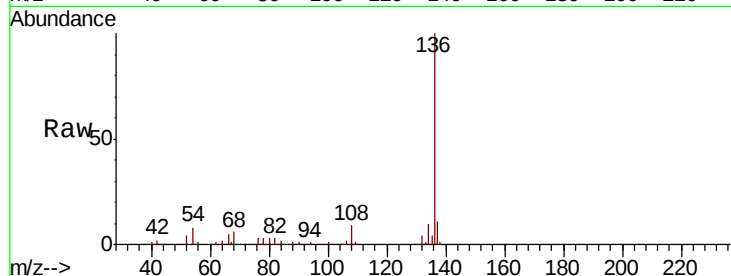


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

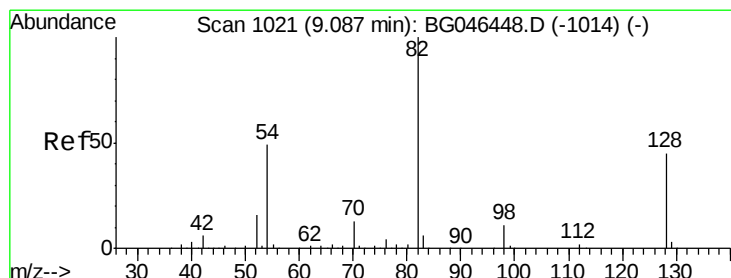
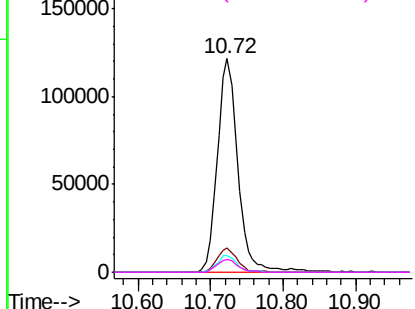



#23
Nitrobenzene-d5
Concen: 79.199 ng
RT: 9.08 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Tgt Ion: 82	Resp:	332744
Ion	Ratio	Lower Upper
82	100	
128	44.6	35.7 53.5
54	47.7	39.4 59.0

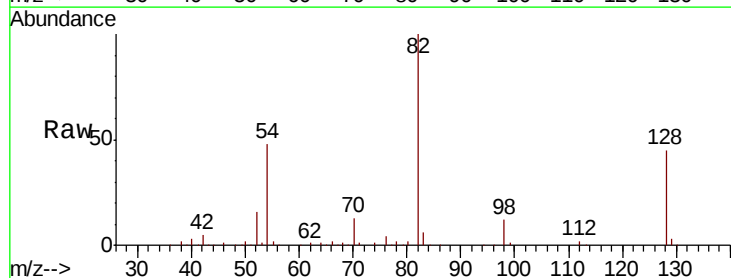

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

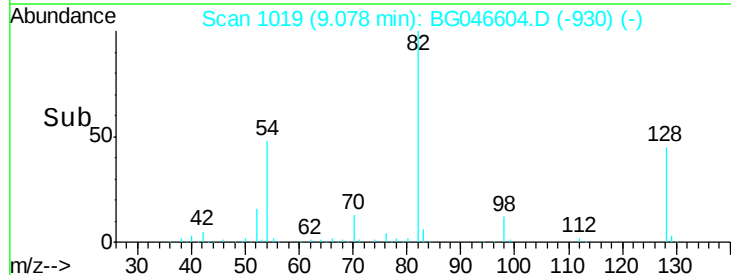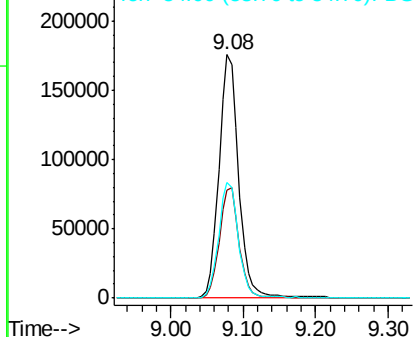



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.55 min Scan# 1951

Delta R.T. -0.01 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30

Instrument :

BNA_G

ClientSampleId :

PB131580BL


Tot Ion:164 Resp: 171342

Ion Ratio Lower Upper

164 100

162 102.7 83.3 124.9




160 45.4 35.0 52.6

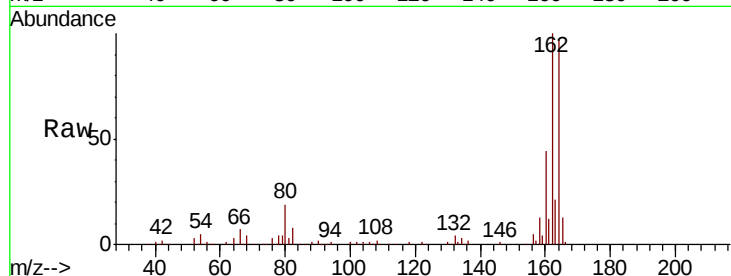

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

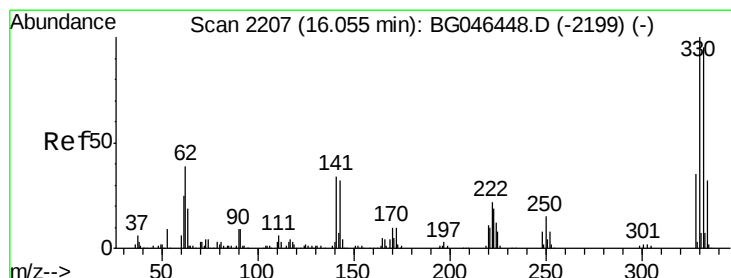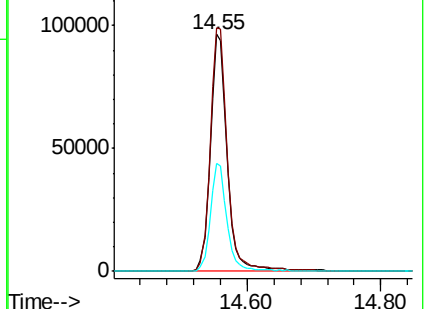

#42

2,4,6-Tribromophenol

Concen: 106.043 ng

RT: 16.05 min Scan# 2205

Delta R.T. -0.00 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30


Tgt Ion:330 Resp: 246186

Ion Ratio Lower Upper

330 100

332 97.7 76.1 114.1



141 32.9 26.1 39.1

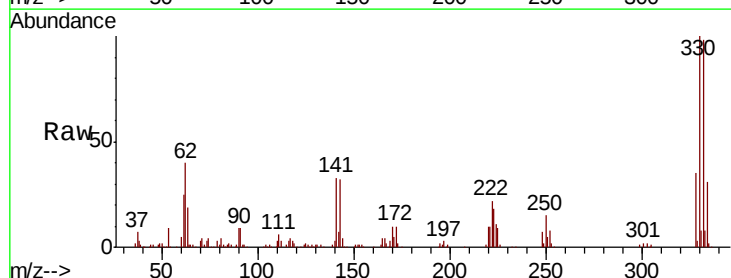


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

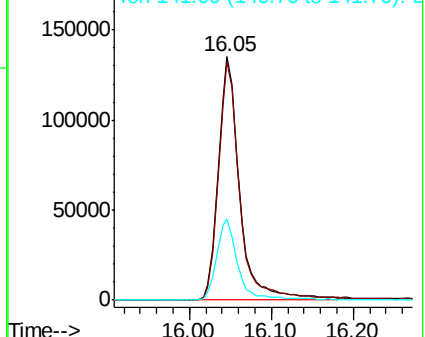


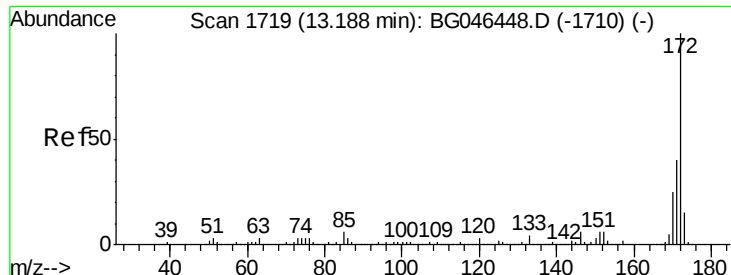




#45
 2-Fluorobiphenyl
 Concen: 82.784 ng
 RT: 13.18 min Scan# 1717
 Delta R.T. -0.01 min
 Lab File: BG046604.D
 Acq: 14 Sep 2020 15:30

Instrument :
 BNA_G
 ClientSampleId :
 PB131580BL

Tot Ion:172 Resp: 929167
 Ion Ratio Lower Upper
 172 100
 171 37.4 31.8 47.6
 170 24.7 20.3 30.5

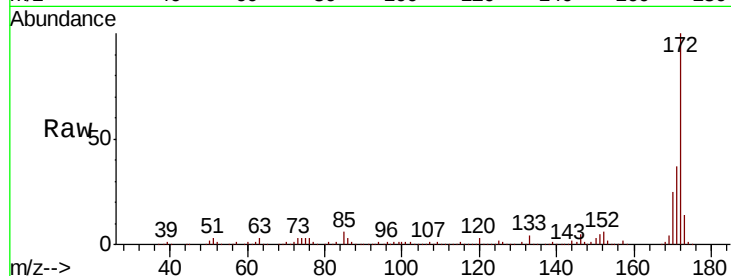


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

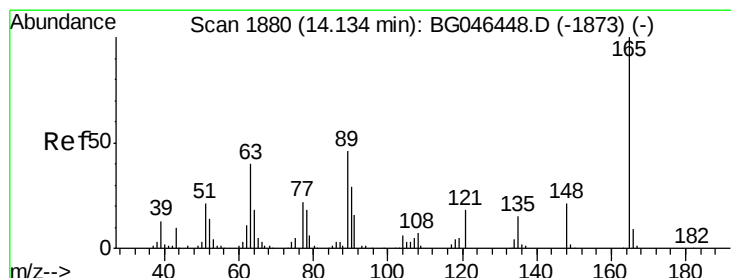
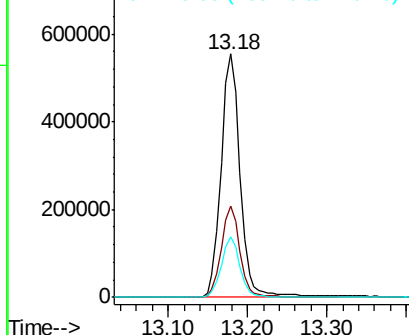



#51
 2,6-Dinitrotoluene
 Concen: 7.513 ng
 RT: 14.55 min Scan# 1951
 Delta R.T. 0.42 min
 Lab File: BG046604.D
 Acq: 14 Sep 2020 15:30

Tgt Ion:165 Resp: 21952
 Ion Ratio Lower Upper
 165 100
 63 0.0 34.2 51.4#
 89 0.0 37.0 55.4#

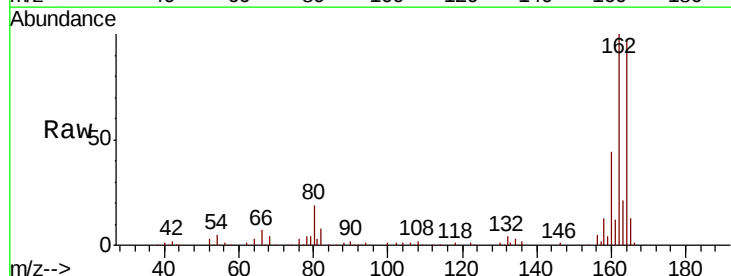

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG
 Ion 89.00 (88.70 to 89.70): BG



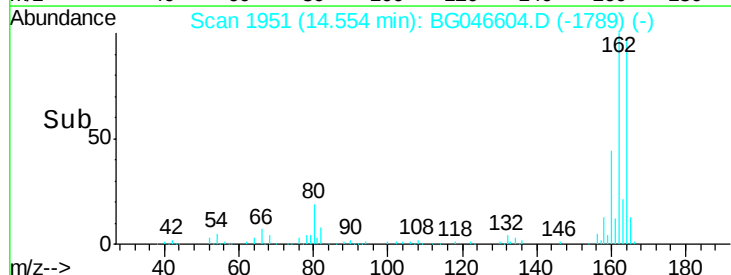
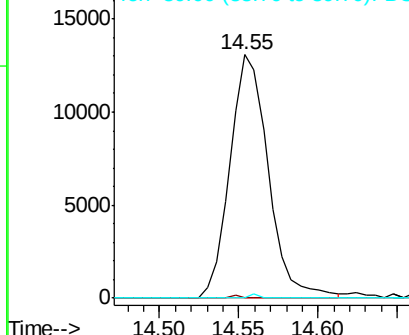


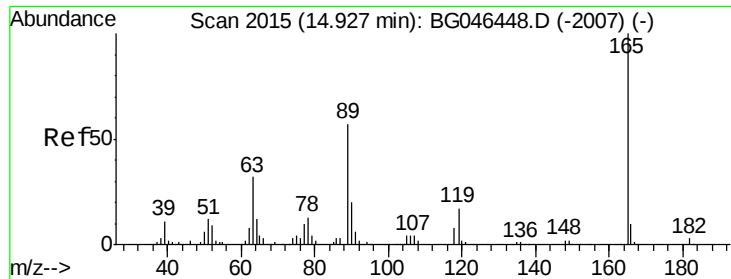

#57
 2,4-Dinitrotoluene
 Concen: 5.269 ng
 RT: 14.55 min Scan# 1951
 Delta R.T. -0.37 min
 Lab File: BG046604.D
 Acq: 14 Sep 2020 15:30




Instrument :
 BNA_G
 ClientSampleId :
 PB131580BL


Tot Ion:165	Resp:	21952
Ion Ratio	Lower	Upper
165	100	
63	0.0	25.4 38.0#
89	0.0	45.9 68.9#
182	0.0	2.3 3.5#

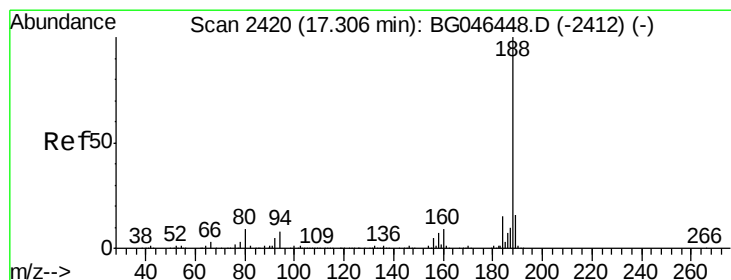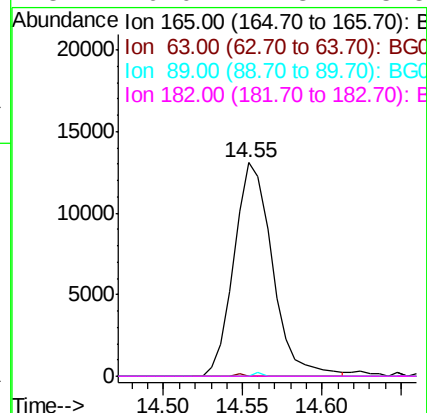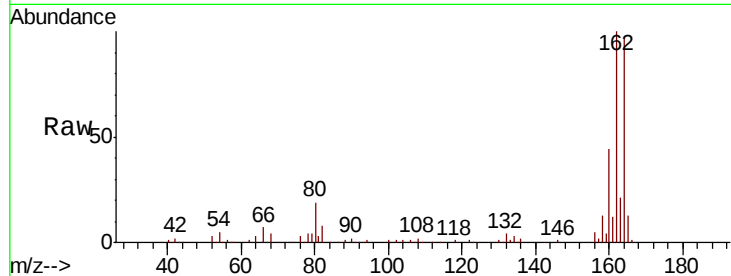

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.30 min Scan# 2418
 Delta R.T. -0.01 min
 Lab File: BG046604.D
 Acq: 14 Sep 2020 15:30

Tgt Ion:188	Resp:	452197
Ion Ratio	Lower	Upper
188	100	
94	7.8	6.3 9.5
80	8.4	6.9 10.3

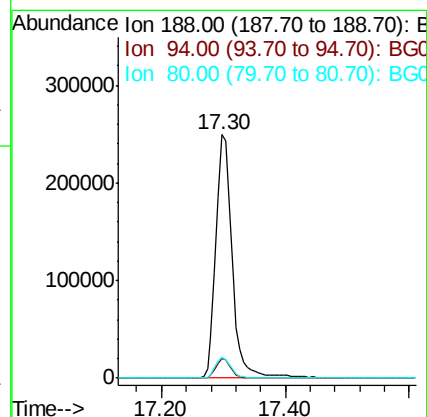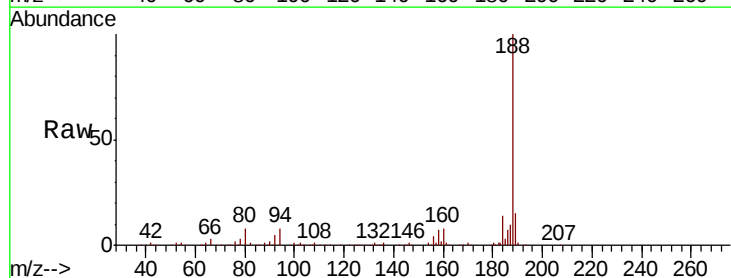


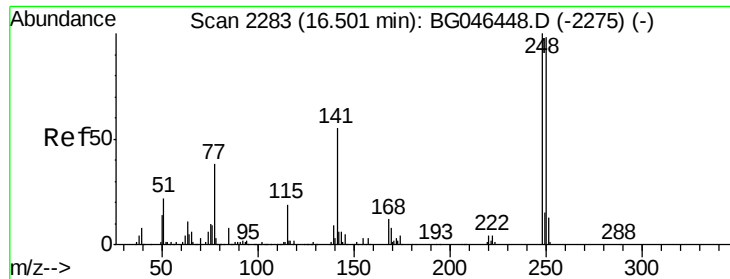




#67
4-Bromophenyl-phenylether
Concen: 3.472 ng
RT: 16.05 min Scan# 2205
Delta R.T. -0.45 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Instrument :
BNA_G
ClientSampleId :
PB131580BL

Tot Ion:248 Resp: 18318
Ion Ratio Lower Upper
248 100
250 199.5 78.6 118.0#
141 448.0 43.9 65.9#

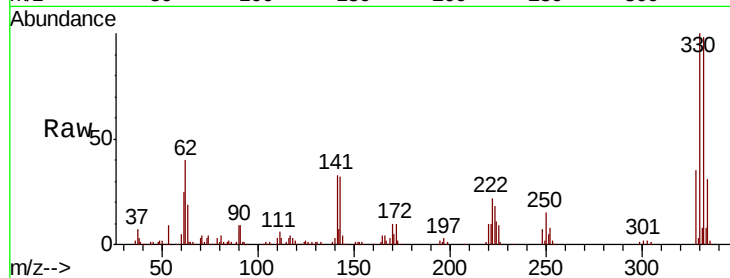


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

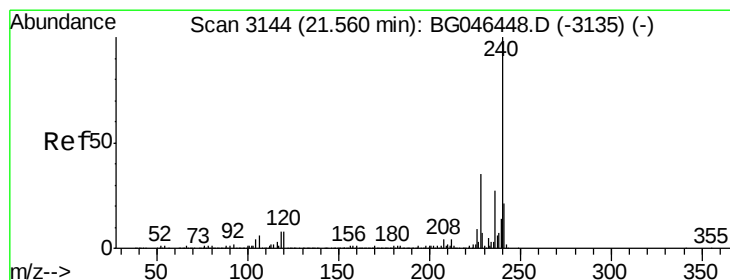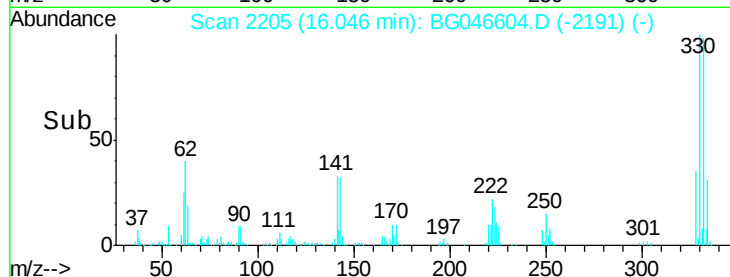
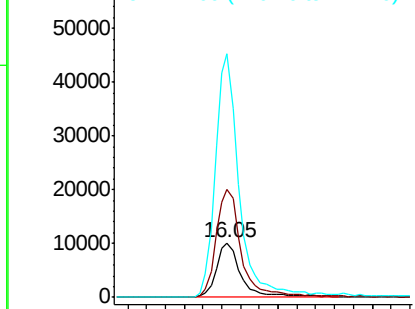


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.55 min Scan# 3141
Delta R.T. -0.01 min
Lab File: BG046604.D
Acq: 14 Sep 2020 15:30

Tgt Ion:240 Resp: 504588
Ion Ratio Lower Upper
240 100
120 8.4 6.6 10.0
236 25.4 21.4 32.2

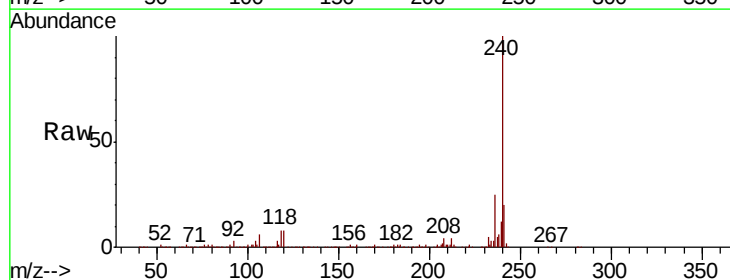

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

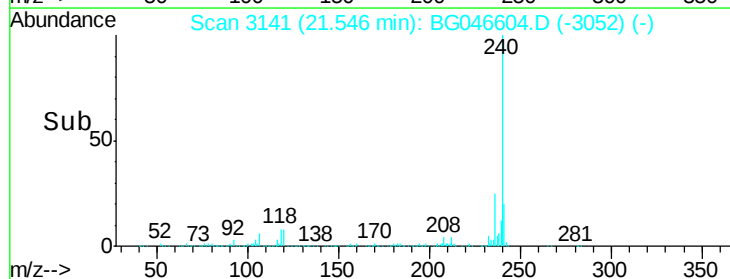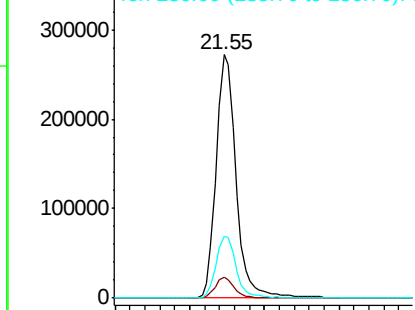



#77

Benzidine

Concen: 2.177 ng

RT: 19.91 min Scan# 2863

Delta R.T. 0.38 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30

Instrument :

BNA_G

ClientSampleId :

PB131580BL


Tot Ion:184 Resp: 25529

Ion Ratio Lower Upper

184 100

185 18.2 11.8 17.8#




183 12.7 10.7 16.1

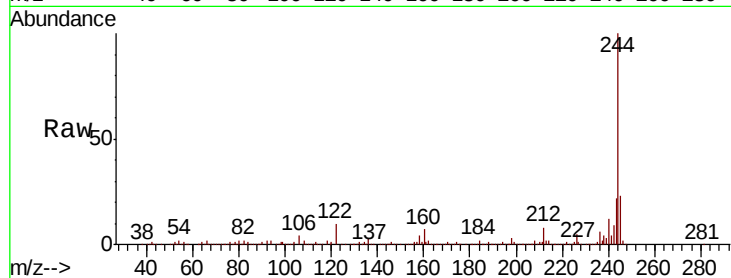

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

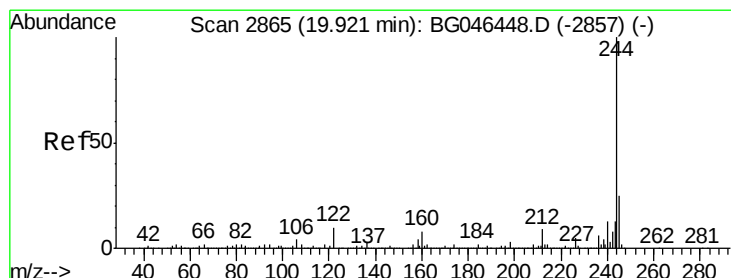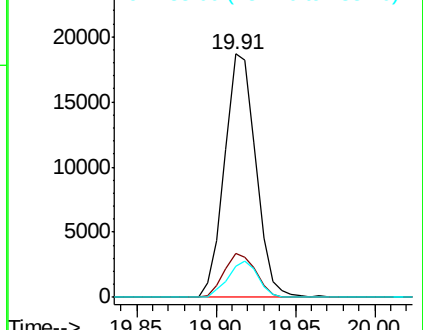

#79

Terphenyl-d14

Concen: 71.503 ng

RT: 19.91 min Scan# 2863

Delta R.T. -0.01 min

Lab File: BG046604.D

Acq: 14 Sep 2020 15:30


Tgt Ion:244 Resp: 1695322

Ion Ratio Lower Upper

244 100

212 8.2 6.9 10.3



122 10.0 8.2 12.4

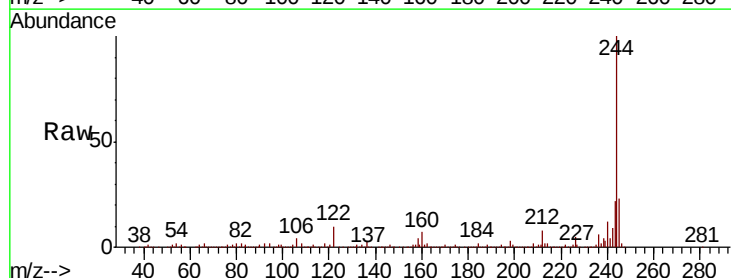


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

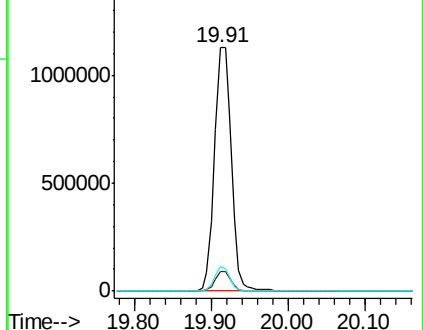




#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.65 min Scan# 3669
 Delta R.T. -0.01 min
 Lab File: BG046604.D
 Acq: 14 Sep 2020 15:30

Instrument :
 BNA_G
 ClientSampleId :
 PB131580BL

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	21.1	17.9	26.9

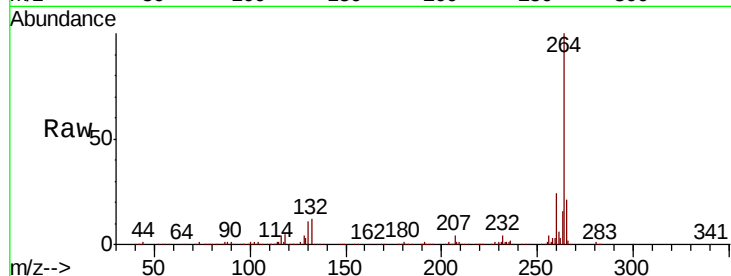

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

