
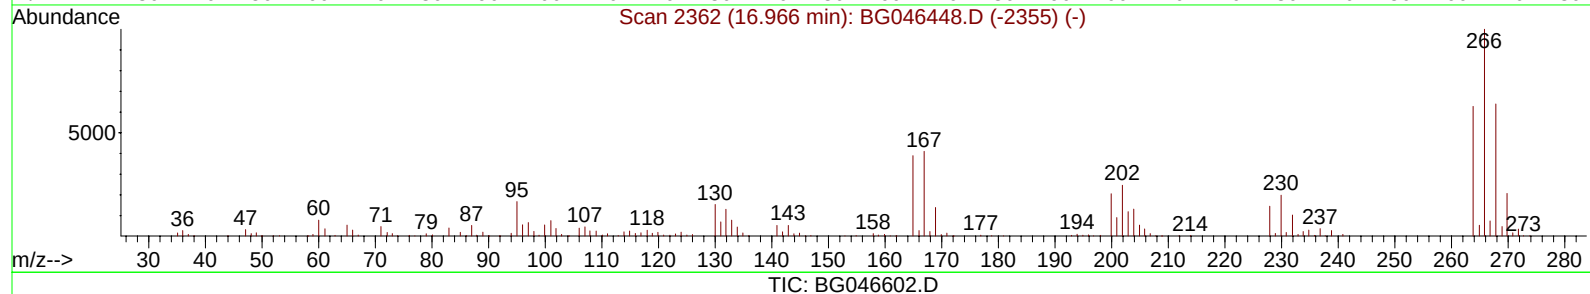
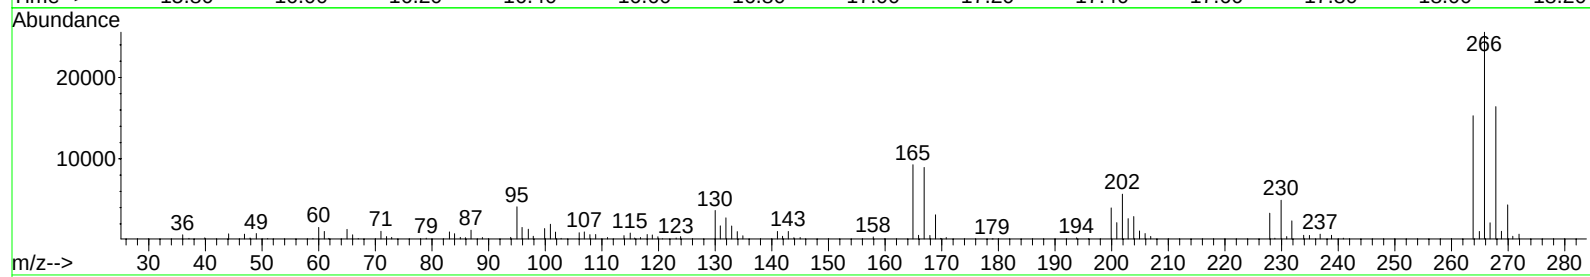


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091420\
Data File : BG046602.D
Acq On : 14 Sep 2020 14:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:28:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

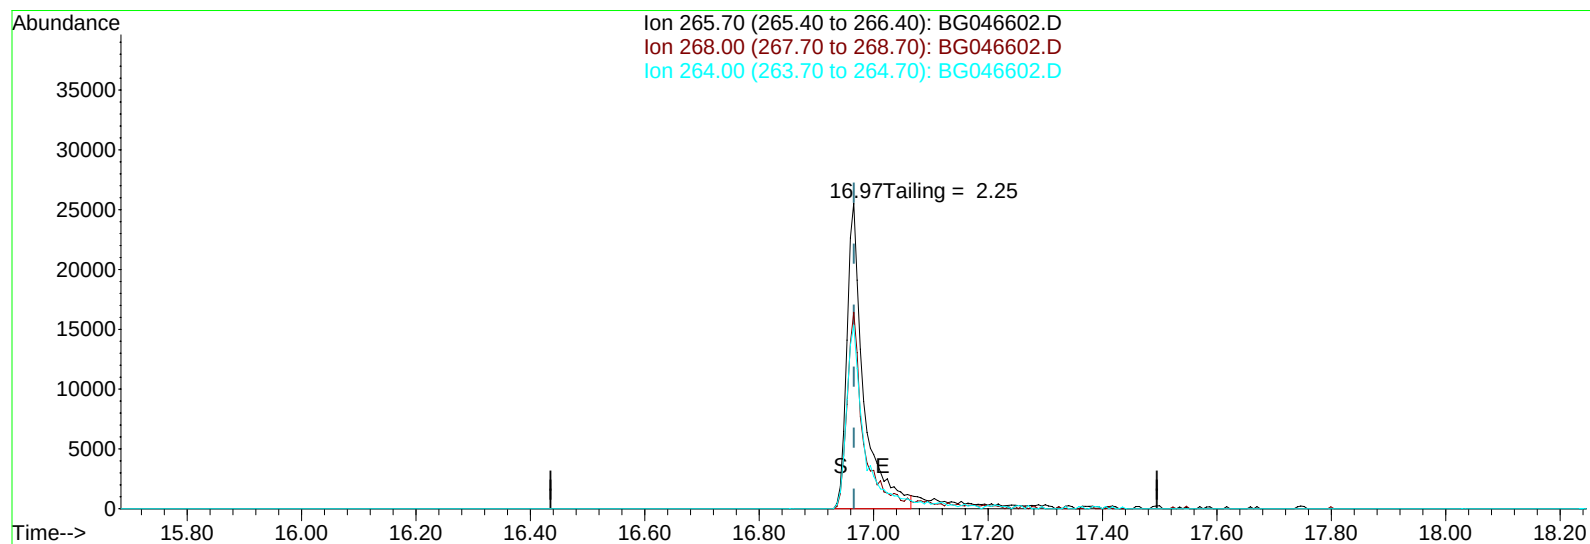

(70) Pentachlorophenol (C)




16.965min (-0.000) 25353.13ng

response 54427

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.26
264.00	62.70	59.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091420\
 Data File : BG046602.D
 Acq On : 14 Sep 2020 14:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:28:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration

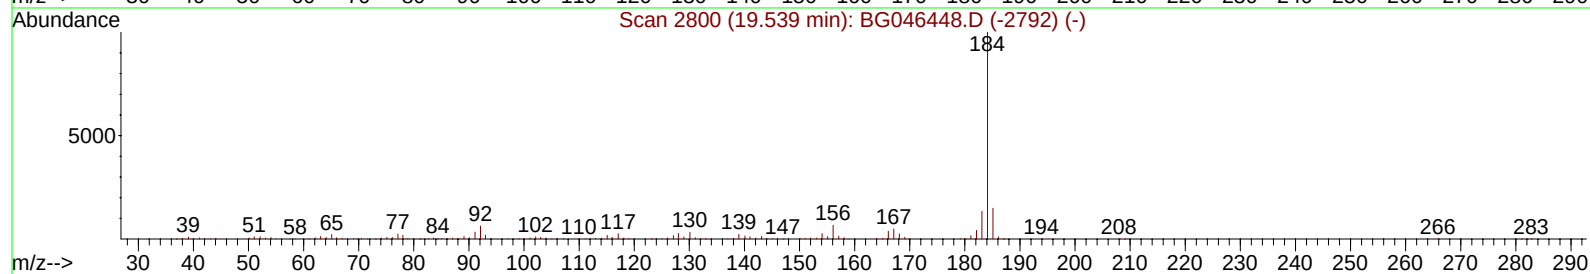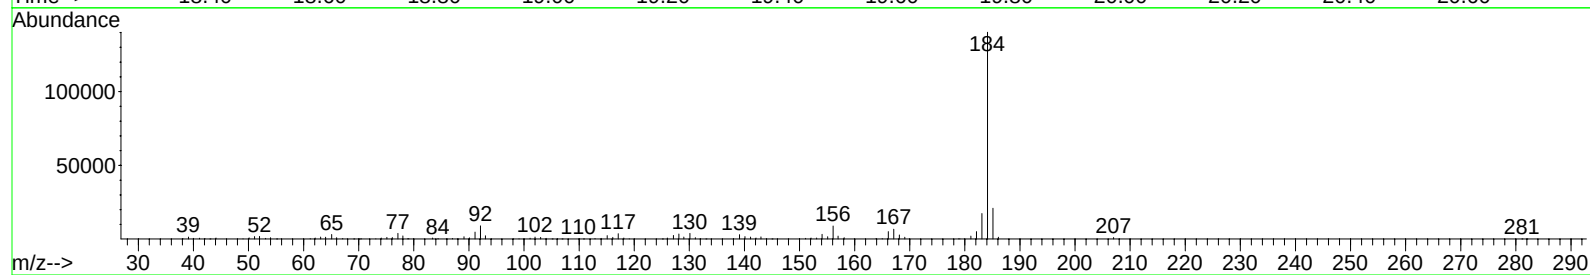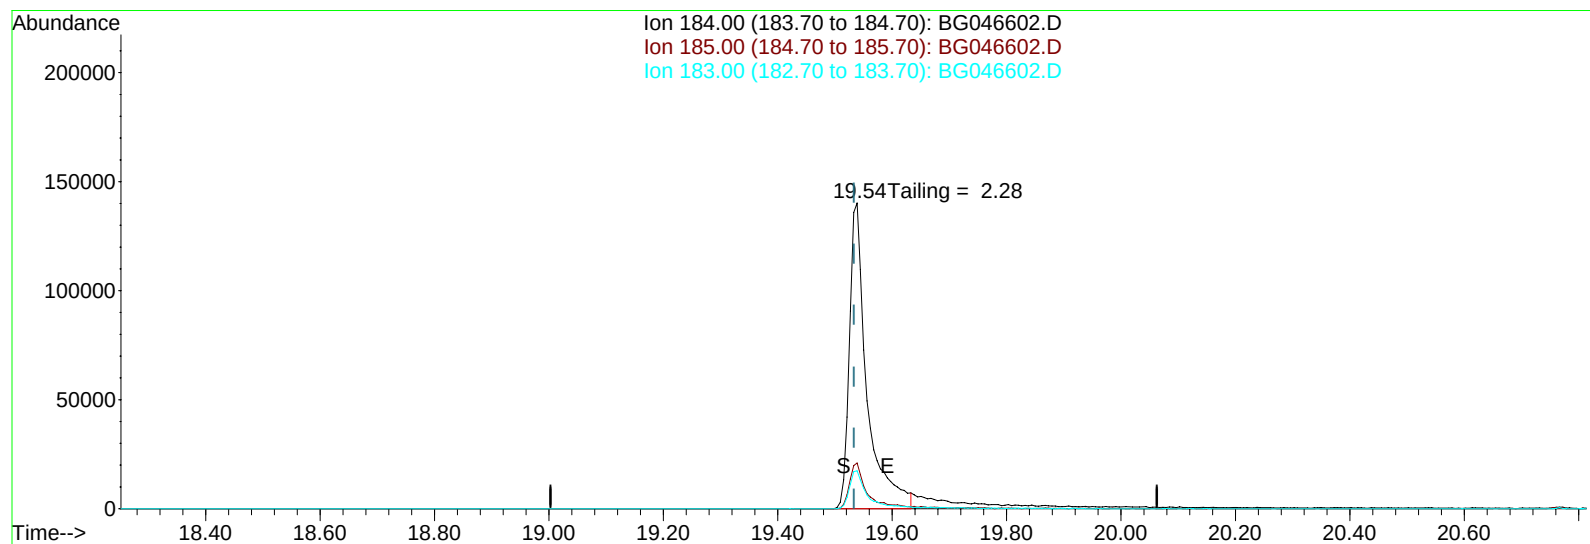

TIC: BG046602.D

(77) Benzidine

19.539min (+0.006) 0.00ng

response 323203

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.95
183.00	13.40	12.40
0.00	0.00	0.00