
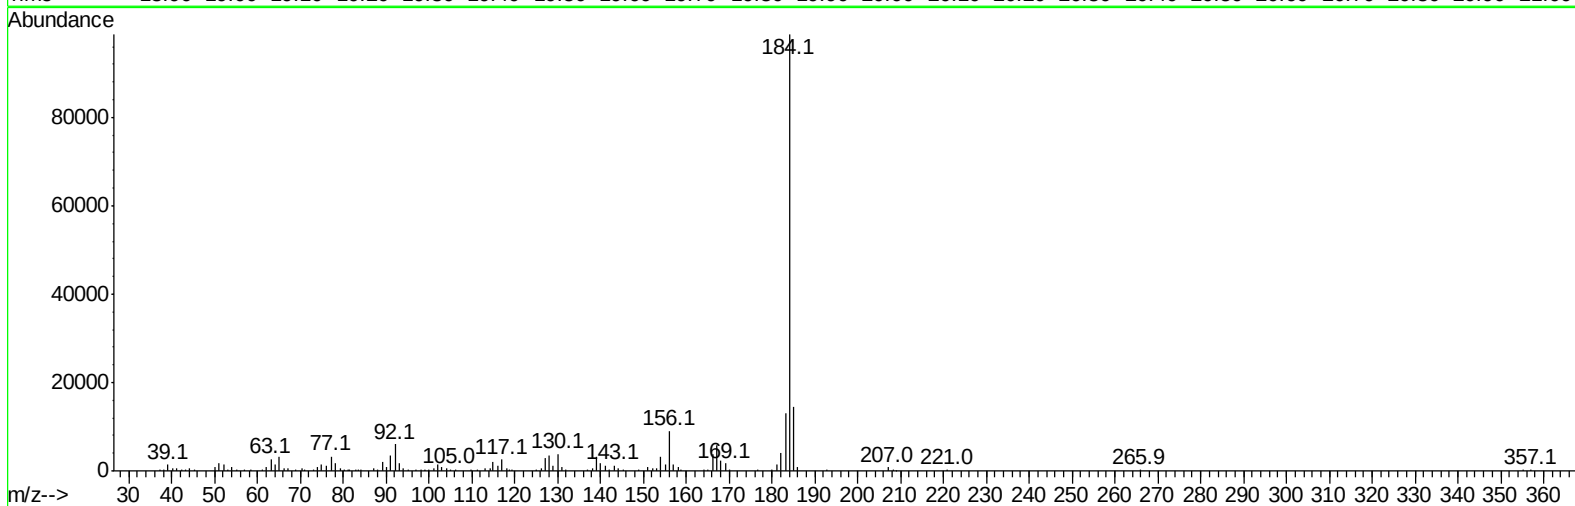


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091517\
Data File : BG028766.D
Acq On : 15 Sep 2017 14:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 01:37:00 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

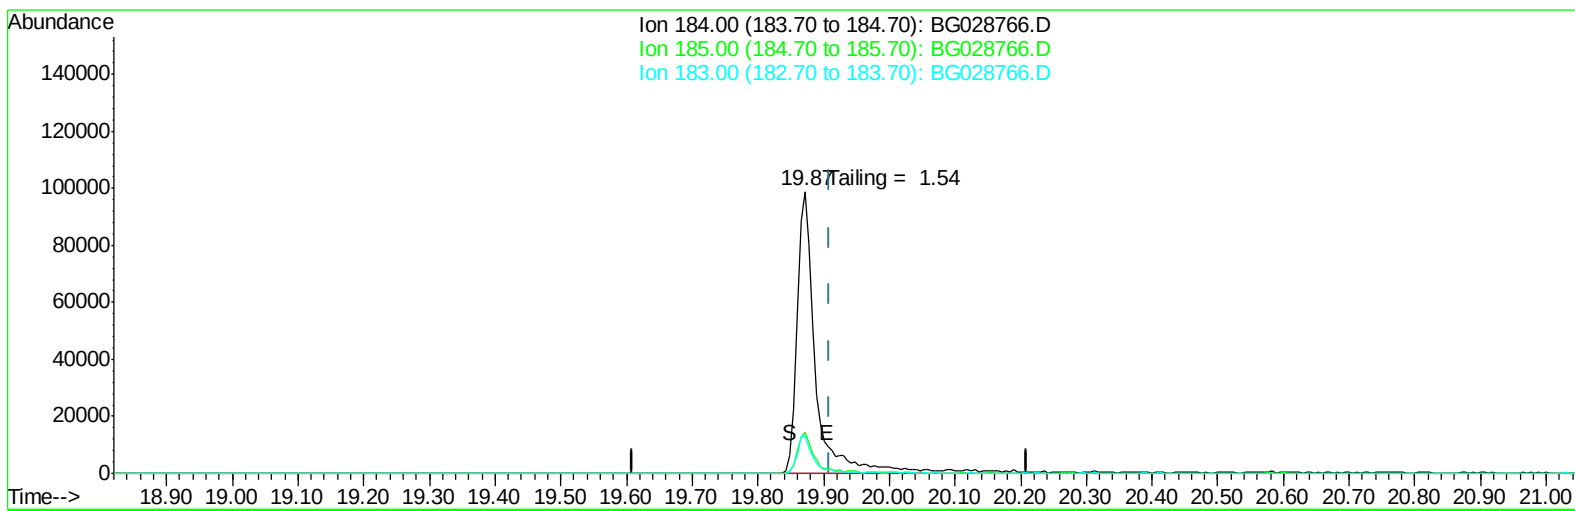

TIC: BG028766.D

(76) Benzidine



19.871min (-0.039) 0.00ng

response 192331

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.59
183.00	13.80	13.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091517\
Data File : BG028766.D
Acq On : 15 Sep 2017 14:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 01:37:00 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

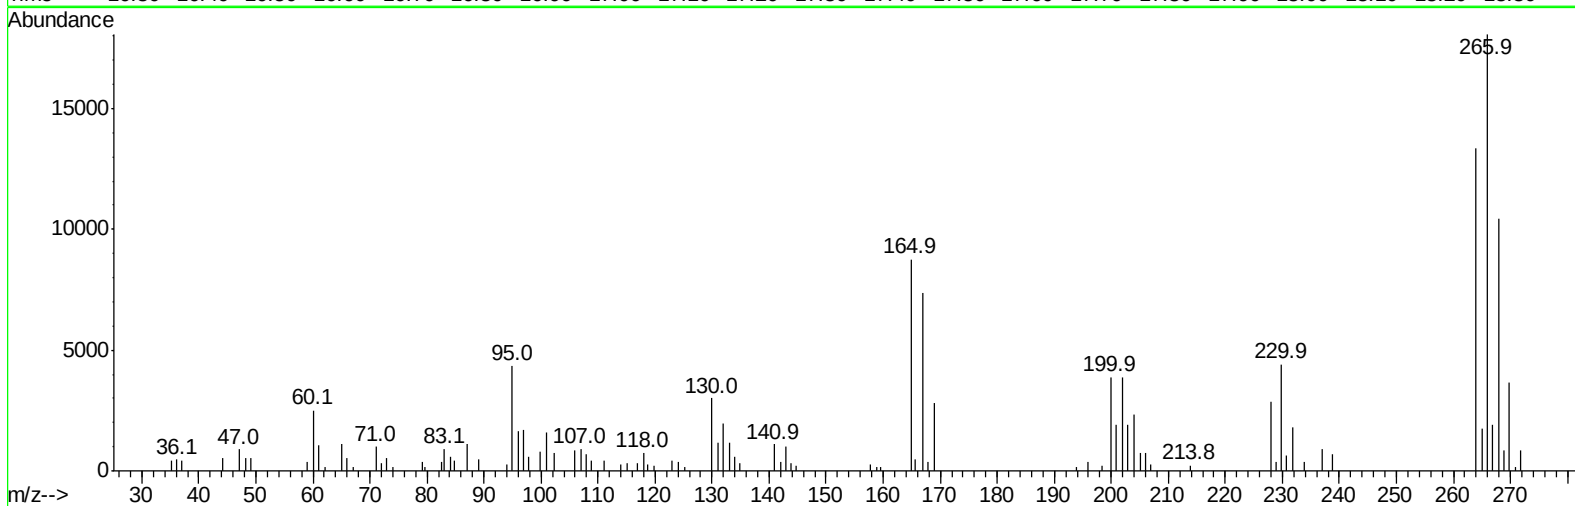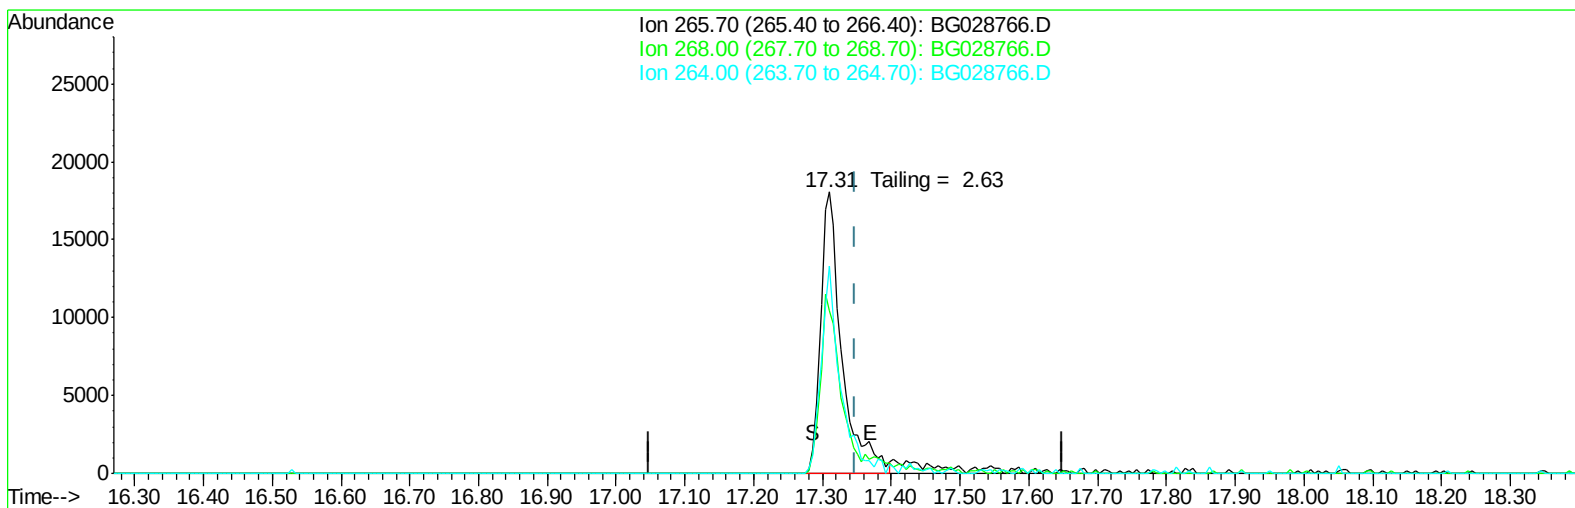

TIC: BG028766.D

(69) Pentachlorophenol (C)

17.310min (-0.039) 108482.77ng m

response 38762

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	57.87
264.00	62.60	73.83
0.00	0.00	0.00