
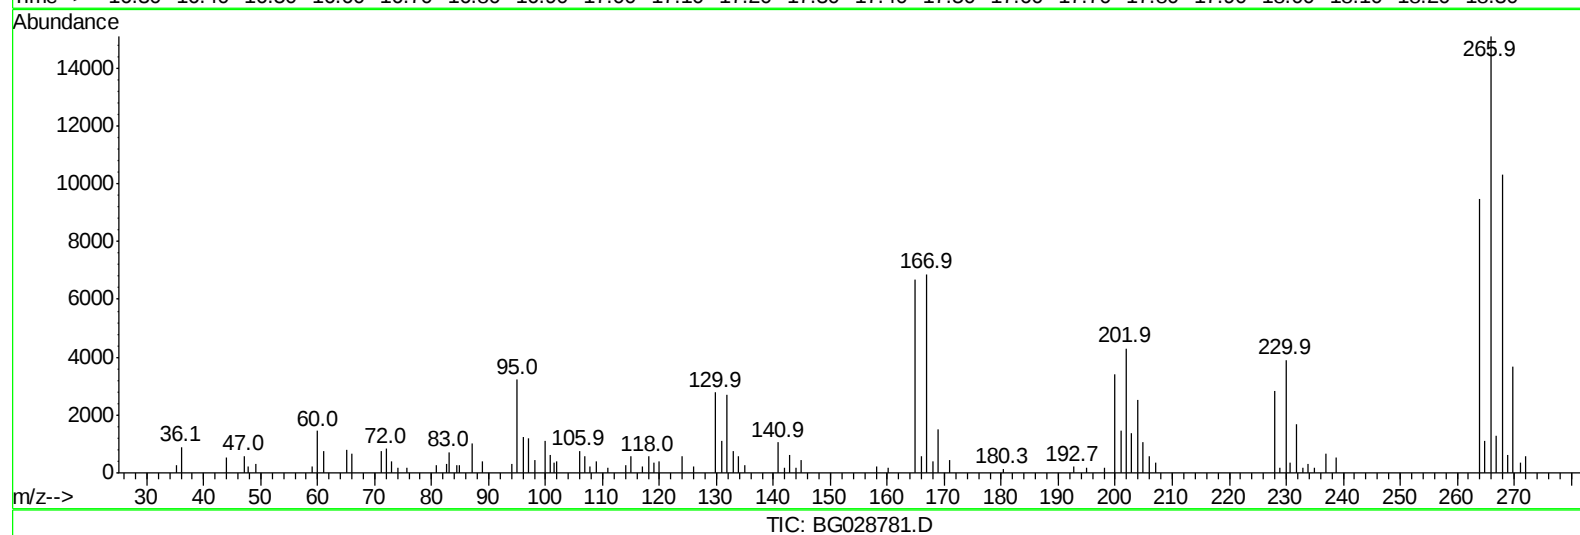


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091517\
Data File : BG028781.D
Acq On : 16 Sep 2017 1:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 01:38:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

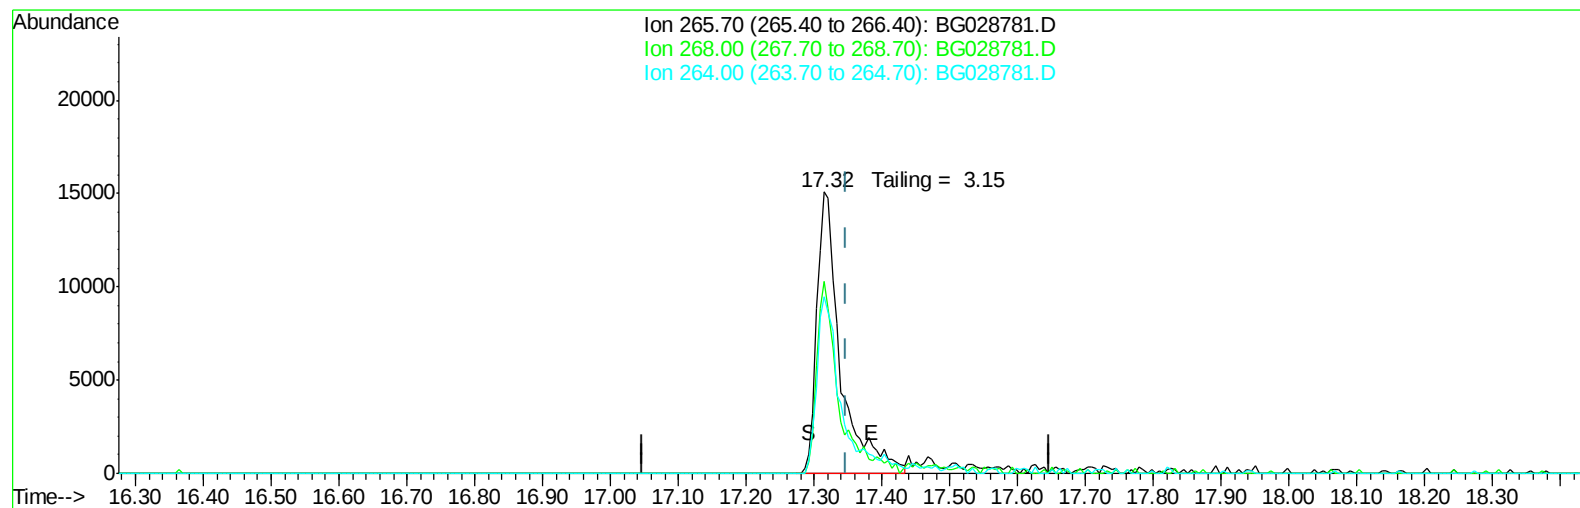

(69) Pentachlorophenol (C)



17.315min (-0.033) 0.00ng

response 36333

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	68.26
264.00	62.60	62.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091517\
Data File : BG028781.D
Acq On : 16 Sep 2017 1:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 01:38:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

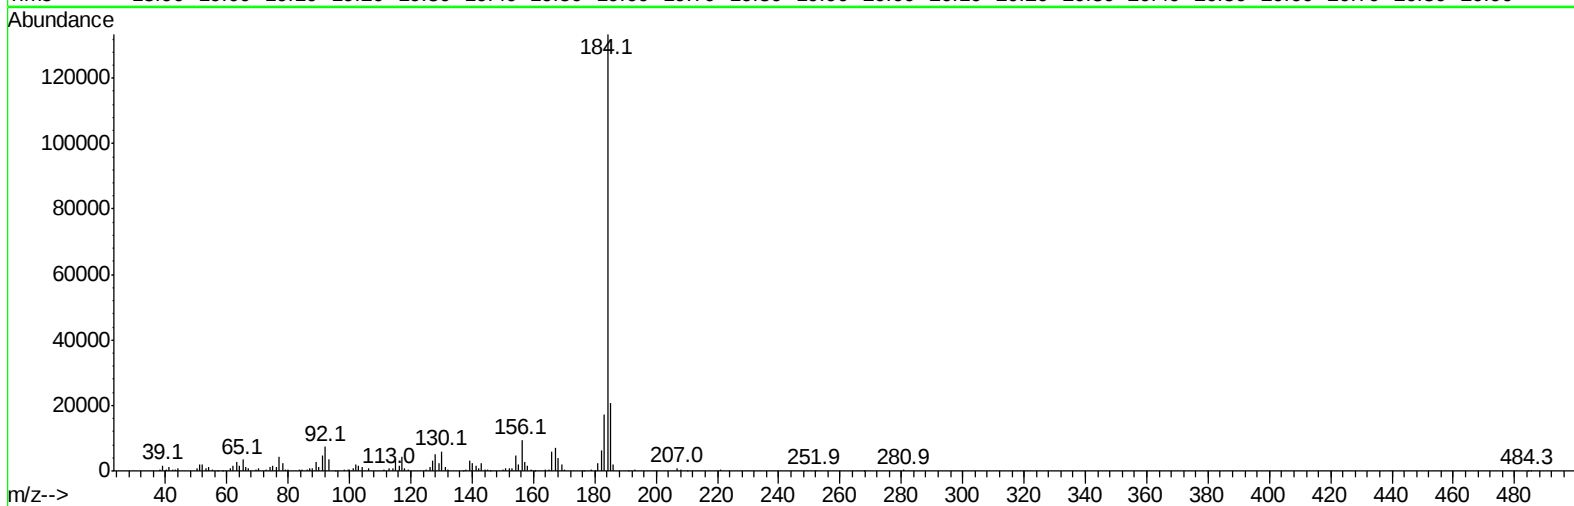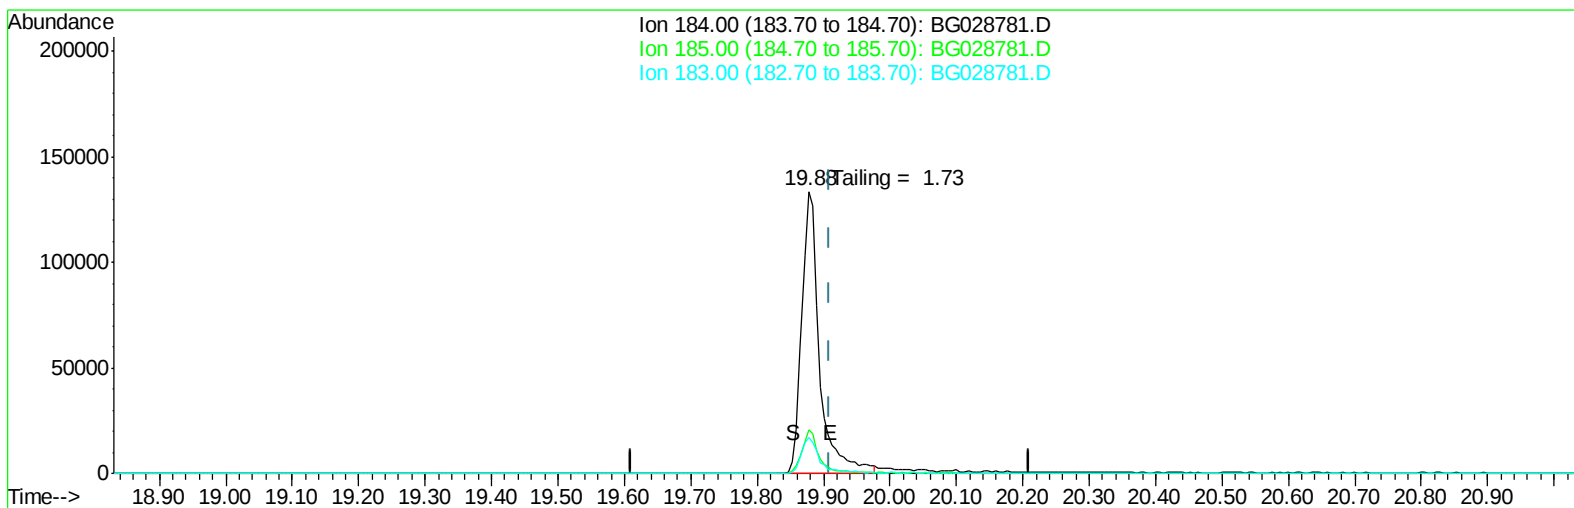

TIC: BG028781.D

(76) Benzidine

19.877min (-0.033) 169863.79ng

response 251083

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.53
183.00	13.80	12.81
0.00	0.00	0.00