


Data Path : Z:\HPCHEM1\BNA_G\Data\BG091517\
 Data File : BG028766.D
 Acq On : 15 Sep 2017 14:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

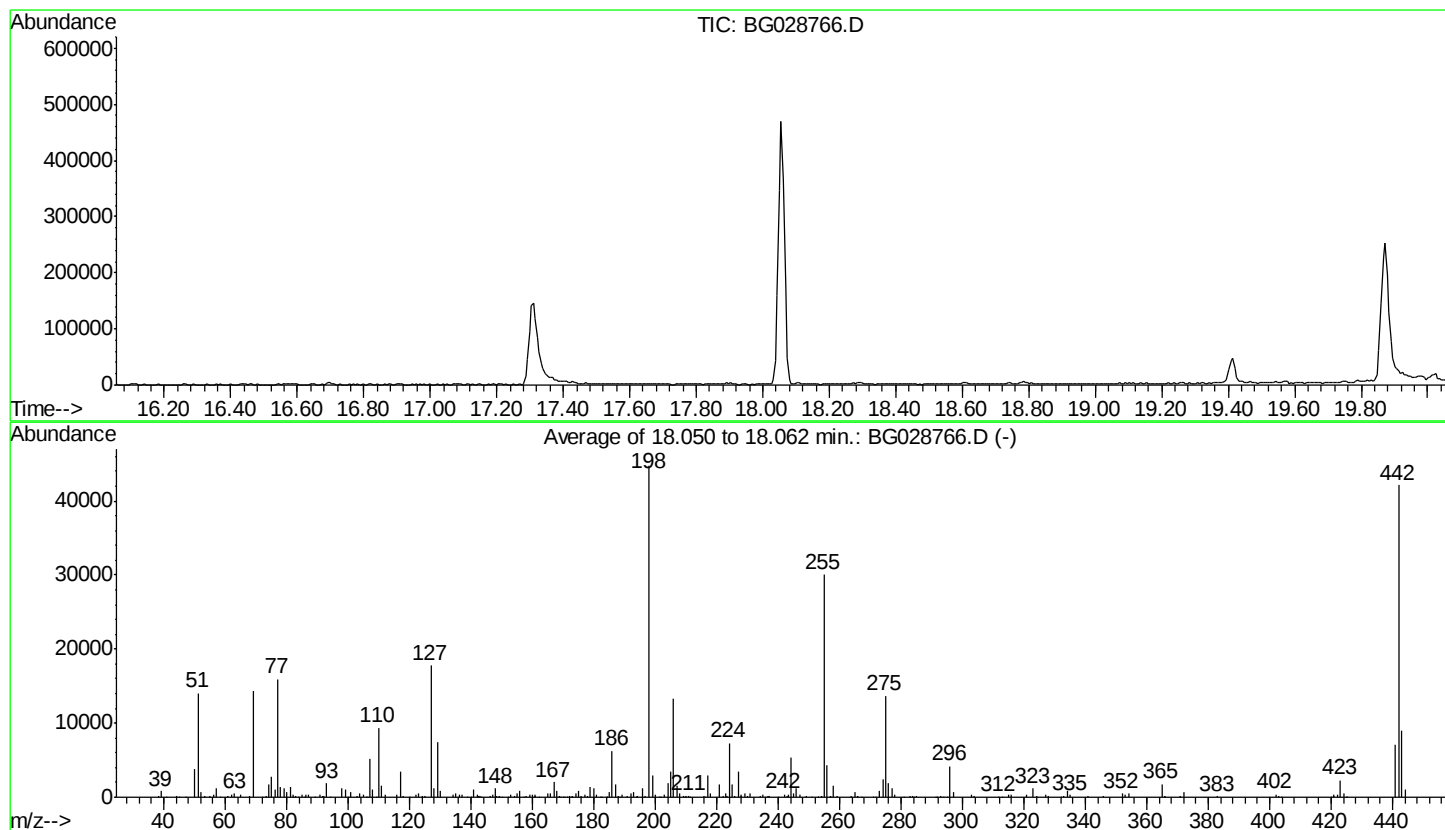

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	14038	PASS
68	69	0.00	2	0.8	112	PASS
69	198	0.00	100	31.9	14273	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.6	17746	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44757	PASS
199	198	5	9	6.7	2981	PASS
275	198	10	60	30.6	13698	PASS
365	198	1	100	4.0	1791	PASS
441	442	0.01	24	17.0	7157	PASS
442	198	50	100	94.0	42093	PASS
443	442	15	24	21.2	8909	PASS