


Data Path : Z:\HPCHEM1\BNA_G\Data\BG091517\
 Data File : BG028781.D
 Acq On : 16 Sep 2017 1:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

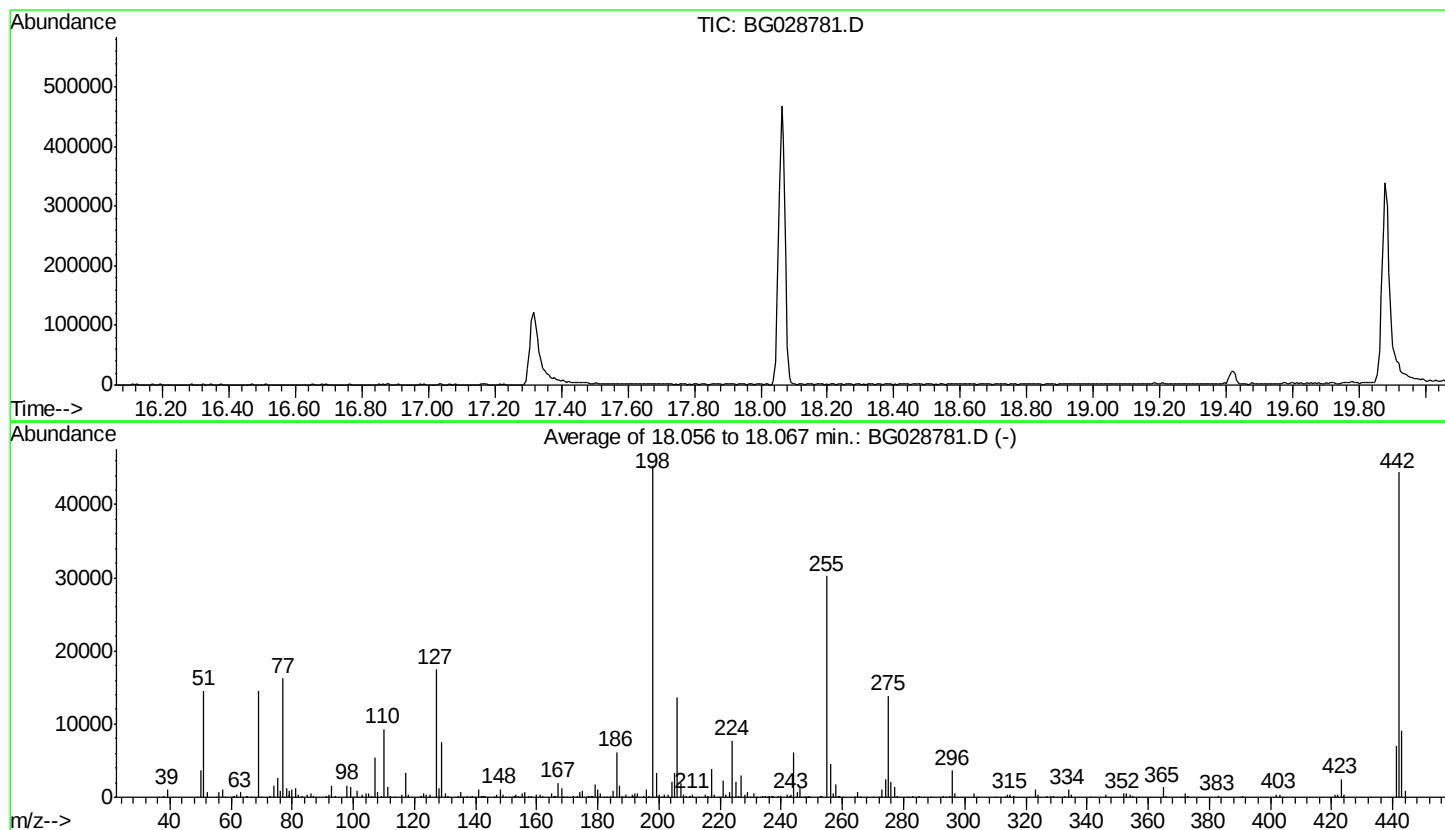

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	14619	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	14549	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	38.6	17493	PASS
197	198	0.00	2	0.2	106	PASS
198	198	100	100	100.0	45338	PASS
199	198	5	9	7.3	3301	PASS
275	198	10	60	30.5	13835	PASS
365	198	1	100	3.0	1351	PASS
441	442	0.01	24	15.6	6962	PASS
442	198	50	100	98.1	44496	PASS
443	442	15	24	20.3	9032	PASS