
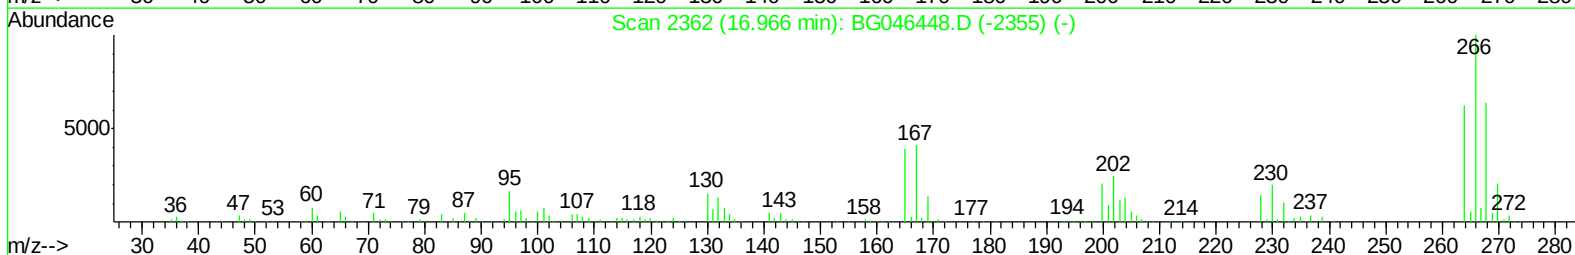
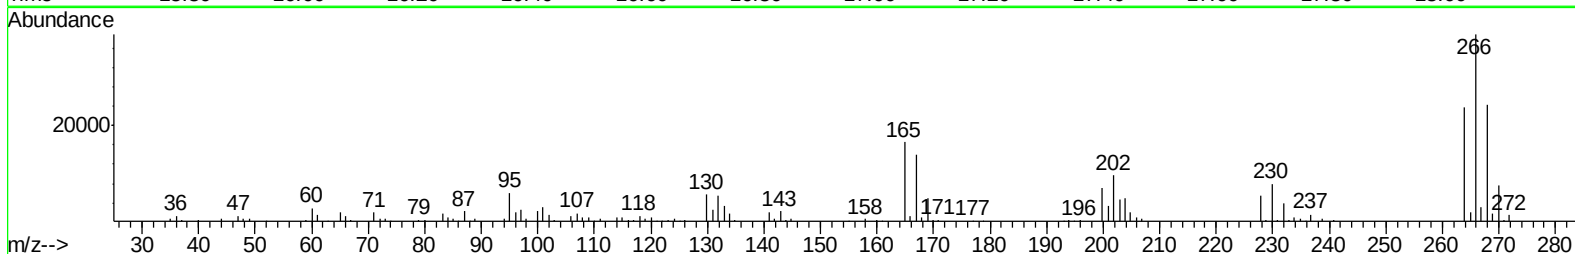


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091520\
 Data File : BG046618.D
 Acq On : 15 Sep 2020 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 04:18:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 15 13:09:36 2020
 Response via : Initial Calibration

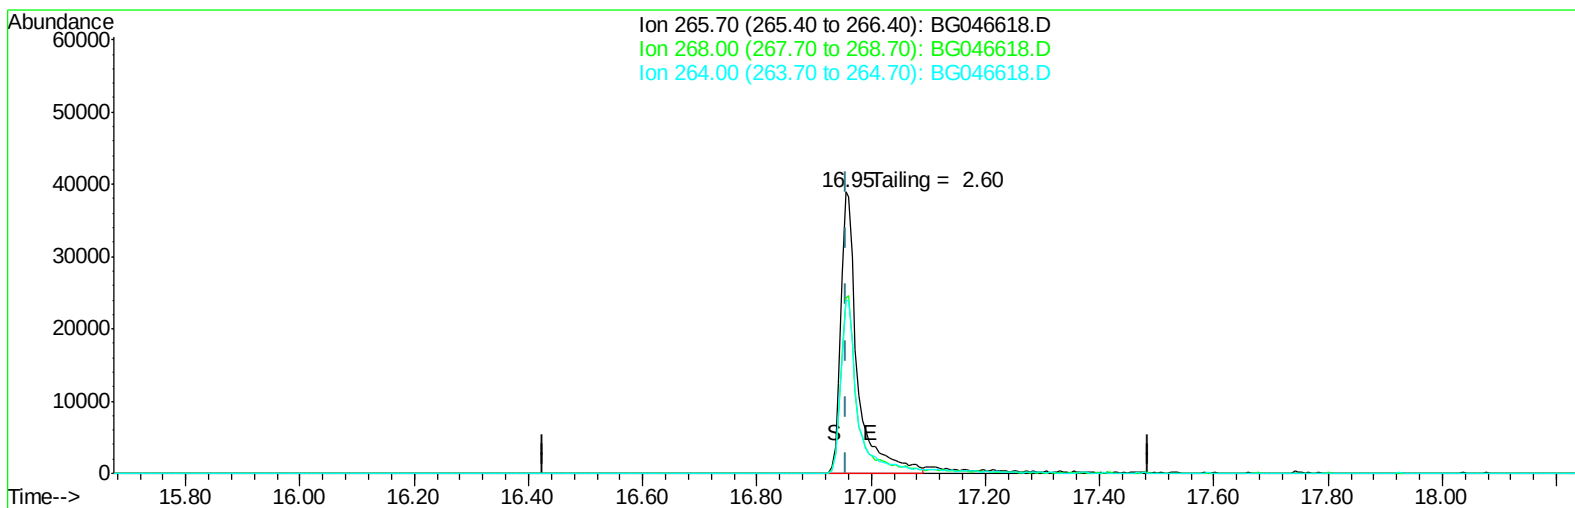

TIC: BG046618.D

(70) Pentachlorophenol (C)




16.955min (-0.002) 30458.05ng

response 80396

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.28
264.00	62.70	61.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091520\
 Data File : BG046618.D
 Acd On : 15 Sep 2020 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 04:18:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 15 13:09:36 2020
 Response via : Initial Calibration

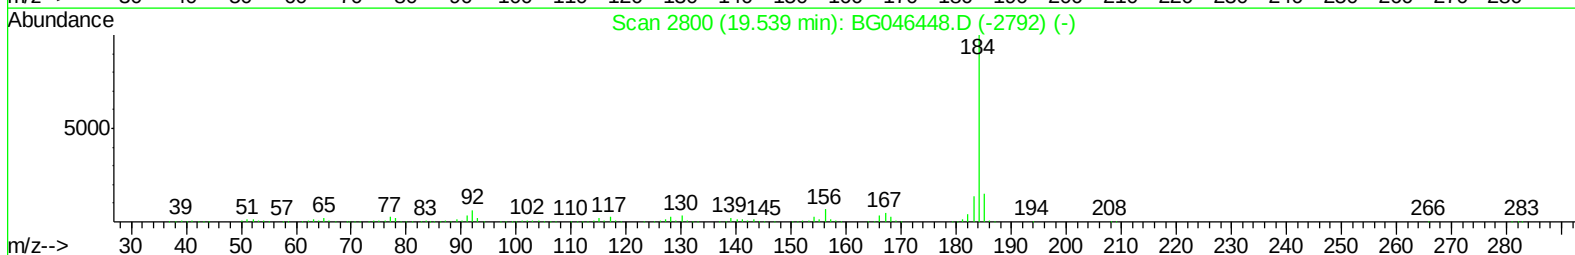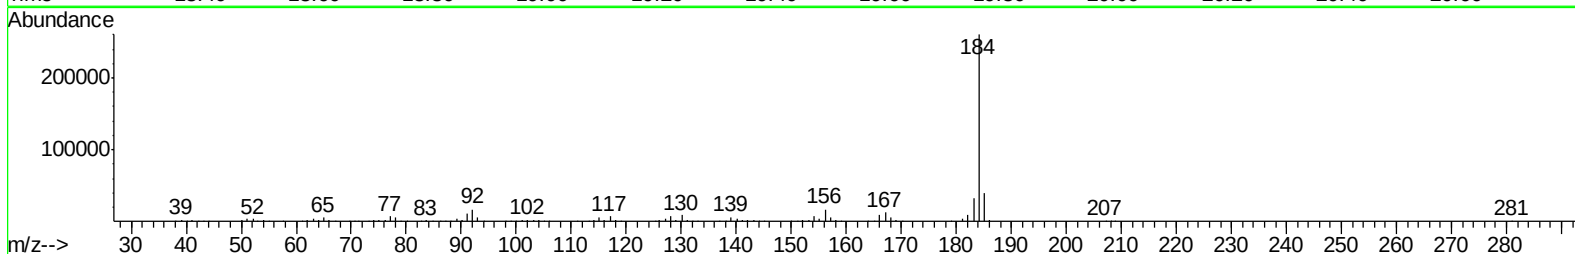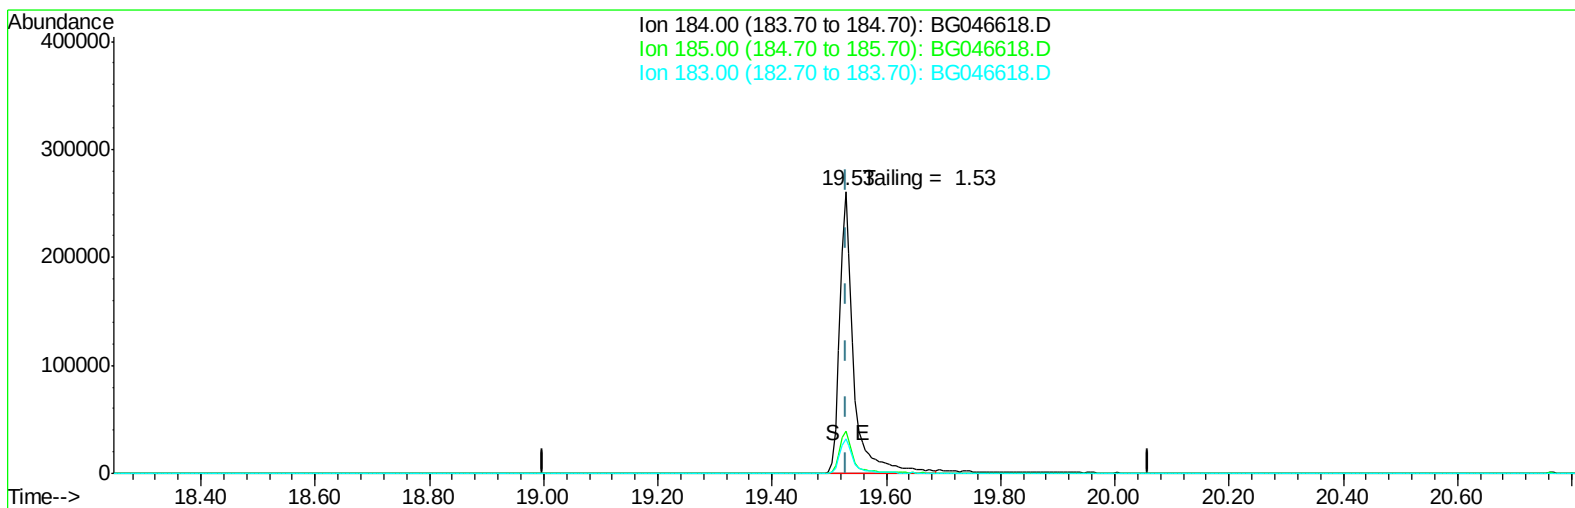

TIC: BG046618.D

(77) Benzidine

19.528min (-0.002) 102557.60ng

response 443261

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.22
183.00	13.40	12.36
0.00	0.00	0.00