


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091520\
 Data File : BG046618.D
 Acq On : 15 Sep 2020 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 15 13:09:36 2020

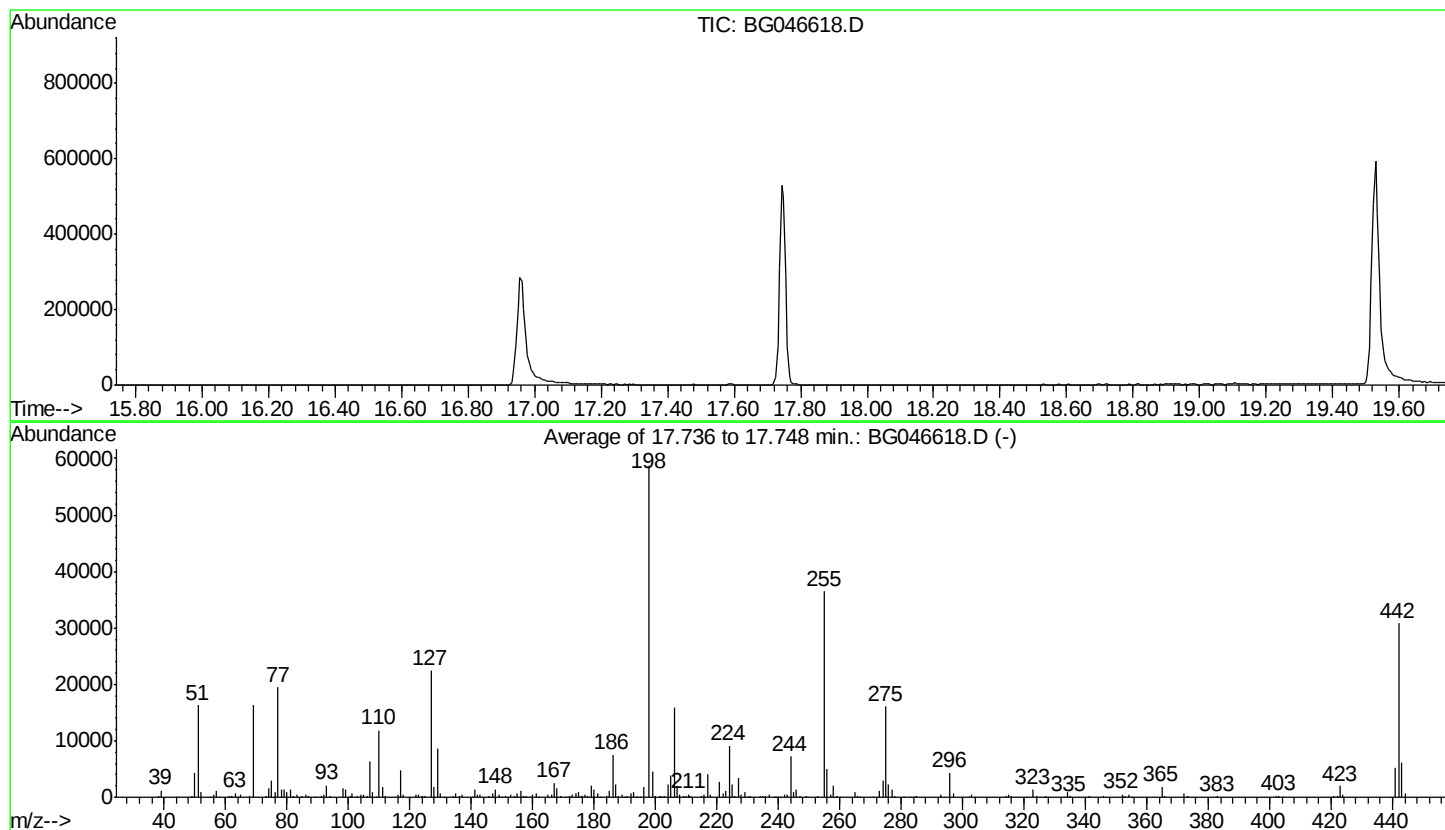

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	16264	PASS
68	69	0.00	2	1.2	189	PASS
69	198	0.00	100	27.8	16304	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.2	22413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58744	PASS
199	198	5	9	7.6	4439	PASS
275	198	10	60	27.4	16099	PASS
365	198	1	100	3.2	1881	PASS
441	198	0.01	100	8.9	5241	PASS
442	198	50	100	52.4	30808	PASS
443	442	15	24	19.5	6018	PASS