
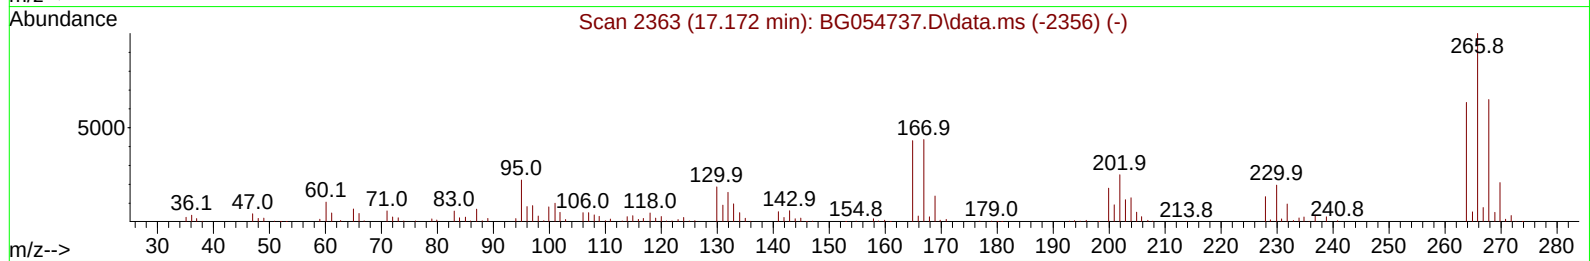
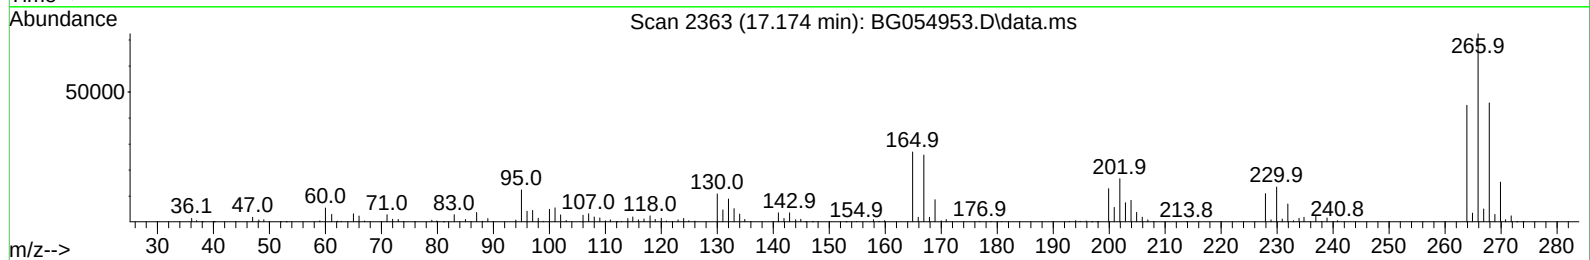


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091522\
 Data File : BG054953.D
 Acq On : 15 Sep 2022 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 12:02:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 03:14:10 2022
 Response via : Initial Calibration

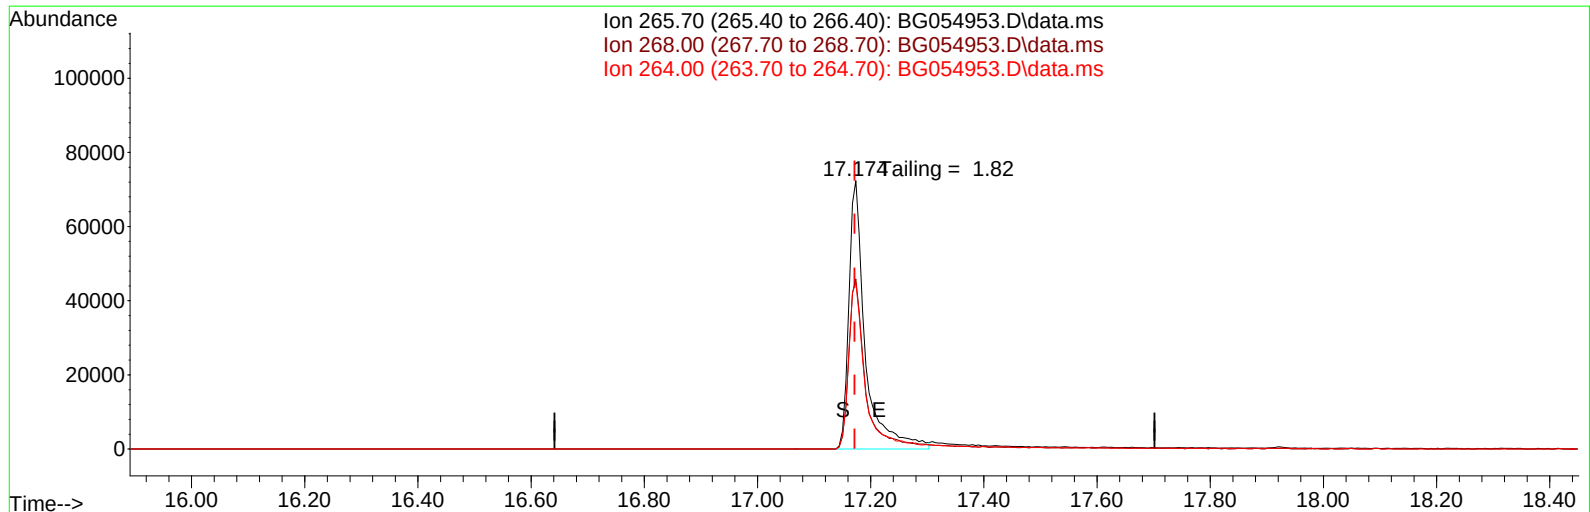

TIC: BG054953.D\data.ms

(70) Pentachlorophenol (C)




17.174min (+ 0.003) 383859.78 ng

response 146729

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.34
264.00	61.70	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091522\
Data File : BG054953.D
Acq On : 15 Sep 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 12:02:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

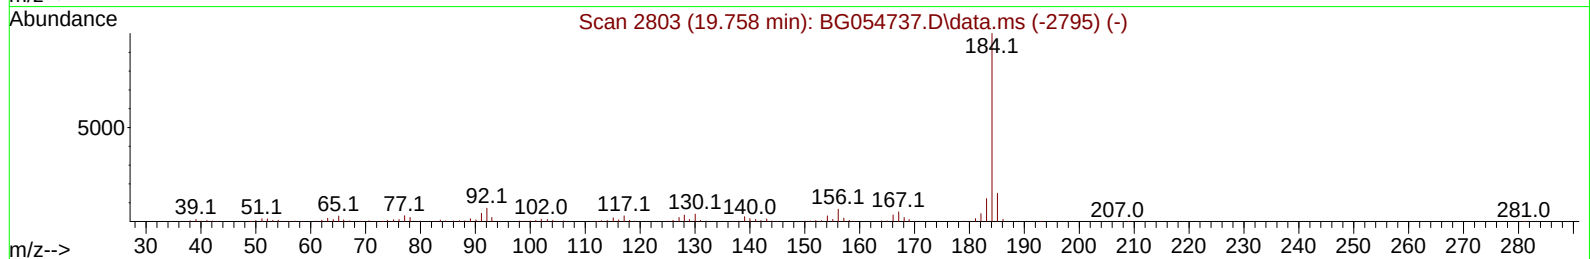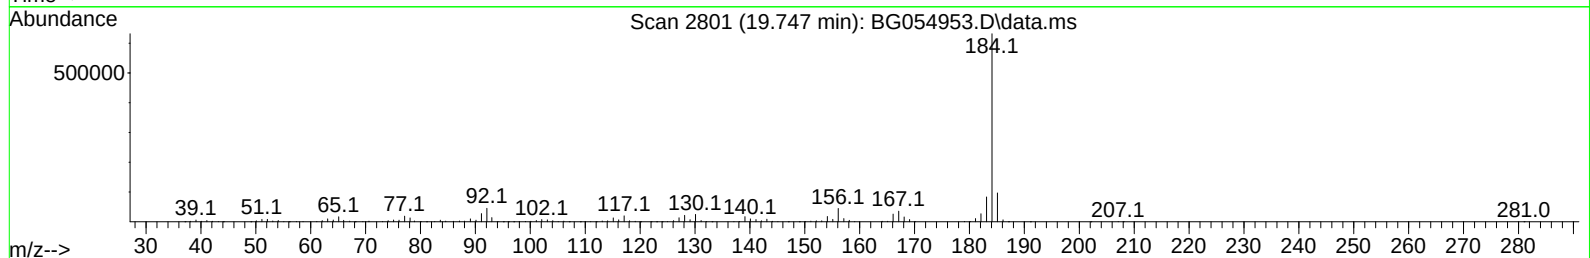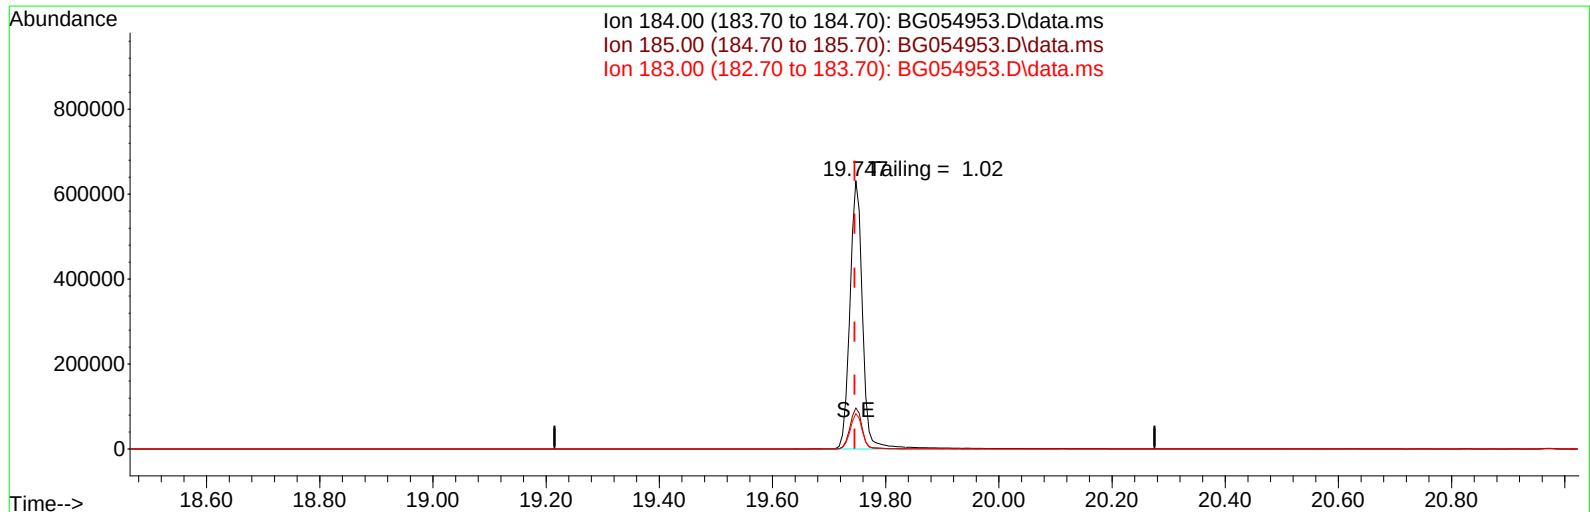

TIC: BG054953.D\data.ms

(77) Benzidine

19.747min (+ 0.003) 10312.03 ng

response 991271

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.31
183.00	12.30	13.18
0.00	0.00	0.00