
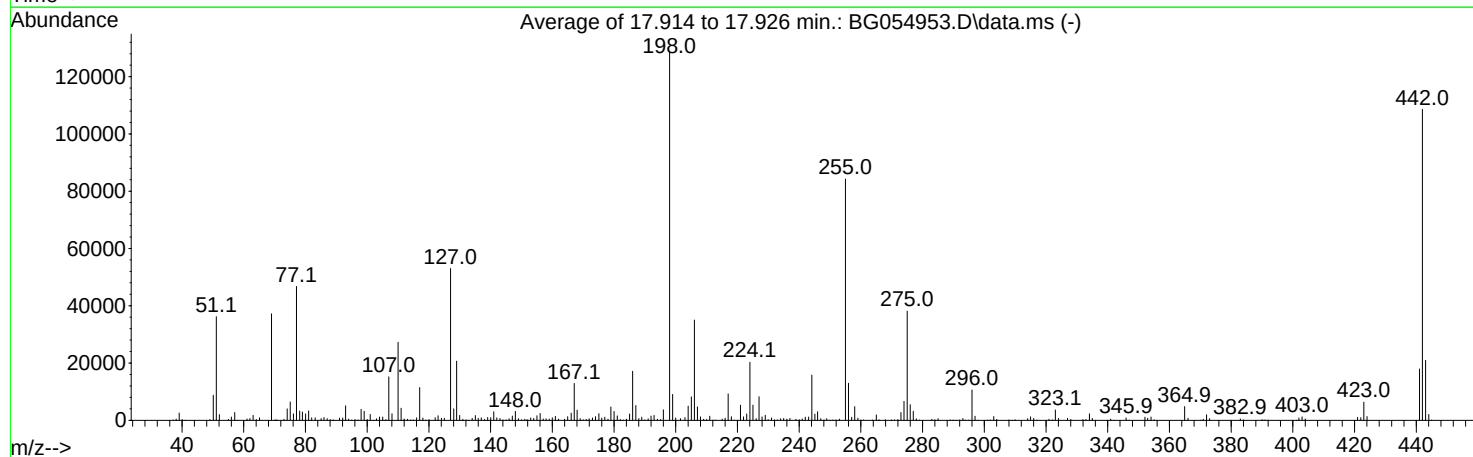


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091522\
 Data File : BG054953.D
 Acq On : 15 Sep 2022 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 15 03:14:10 2022

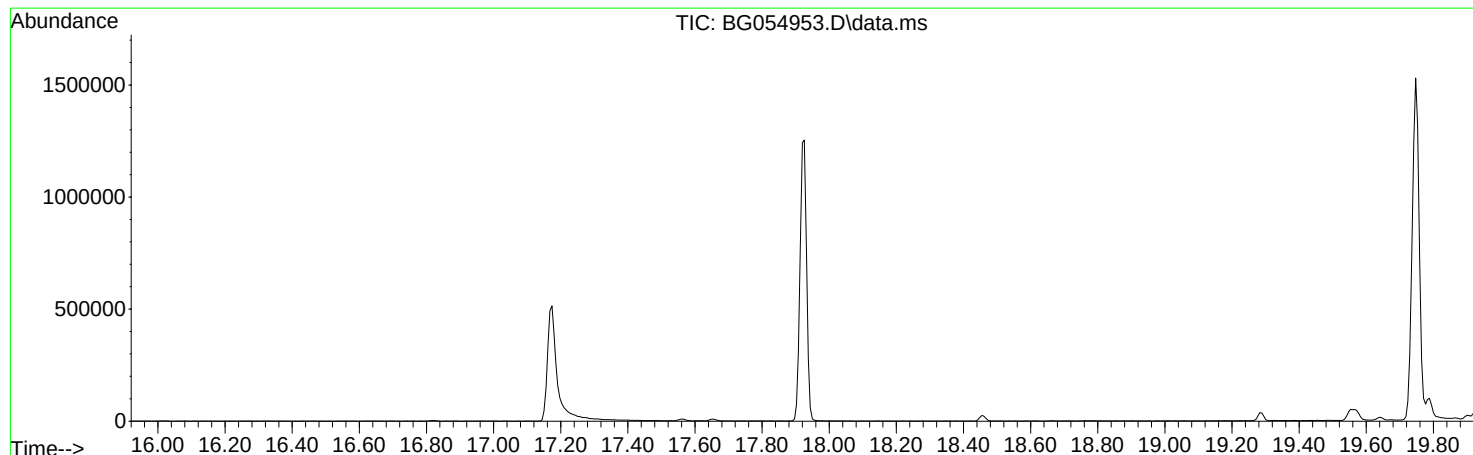




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	36163	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.9	37165	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	41.2	52989	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128461	PASS
199	198	5	9	7.0	9017	PASS
275	198	10	60	29.7	38131	PASS
365	198	1	100	3.7	4794	PASS
441	198	0.01	100	13.9	17917	PASS
442	442	50	100	100.0	108584	PASS
443	442	15	24	19.3	20958	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091522\
Data File : BG054953.D
Acq On : 15 Sep 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:02:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

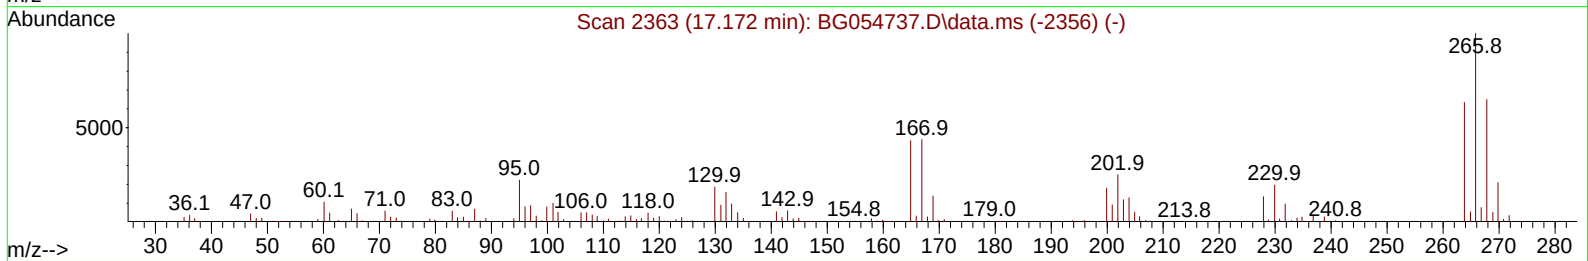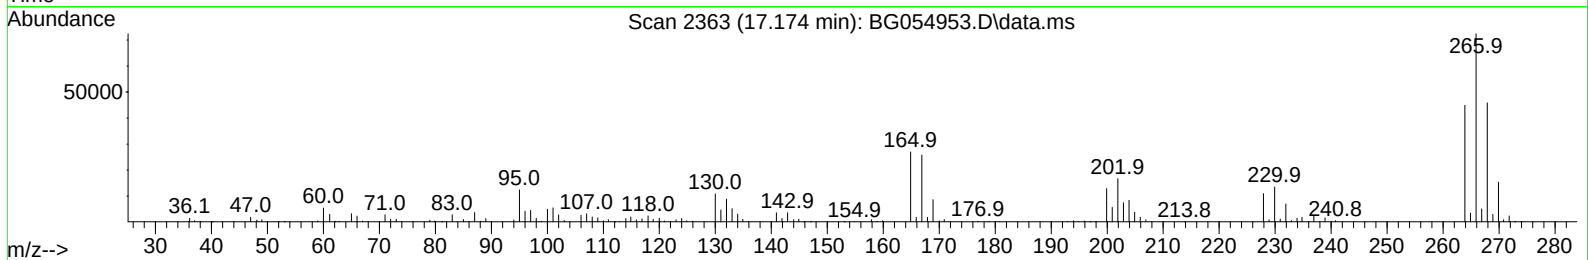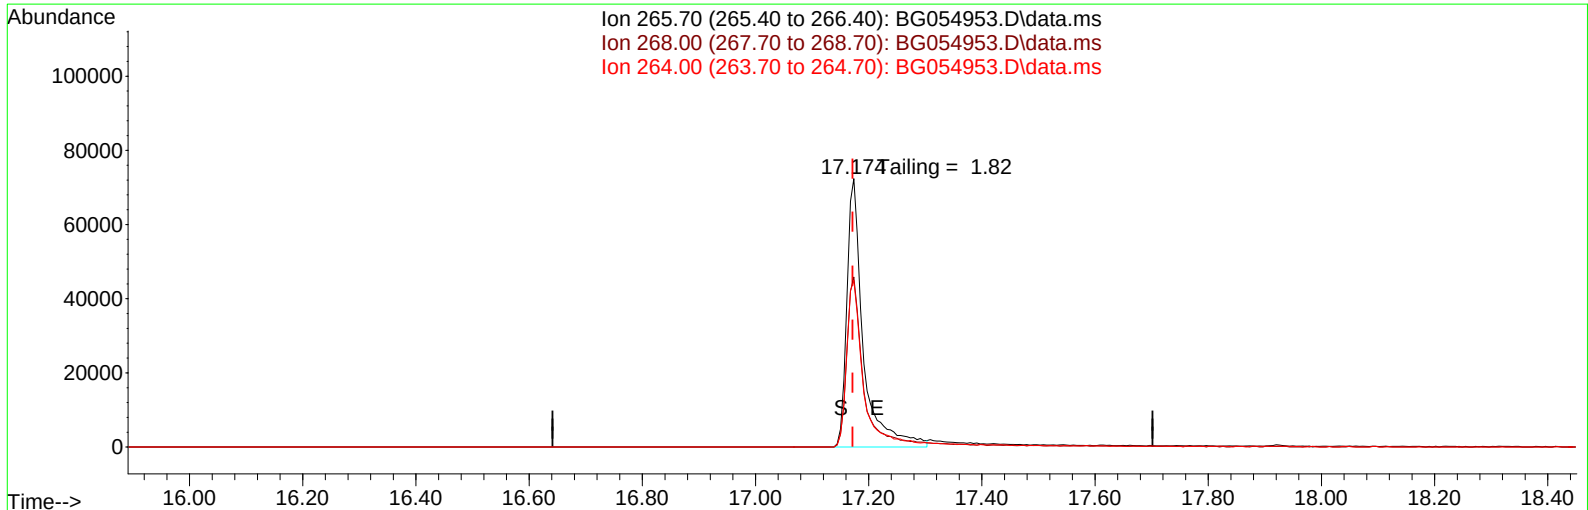

TIC: BG054953.D\data.ms

(70) Pentachlorophenol (C)

17.174min (+ 0.003) 383859.78 ng




response 146729

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.34
264.00	61.70	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091522\
Data File : BG054953.D
Acq On : 15 Sep 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 15 12:02:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 03:14:10 2022
Response via : Initial Calibration

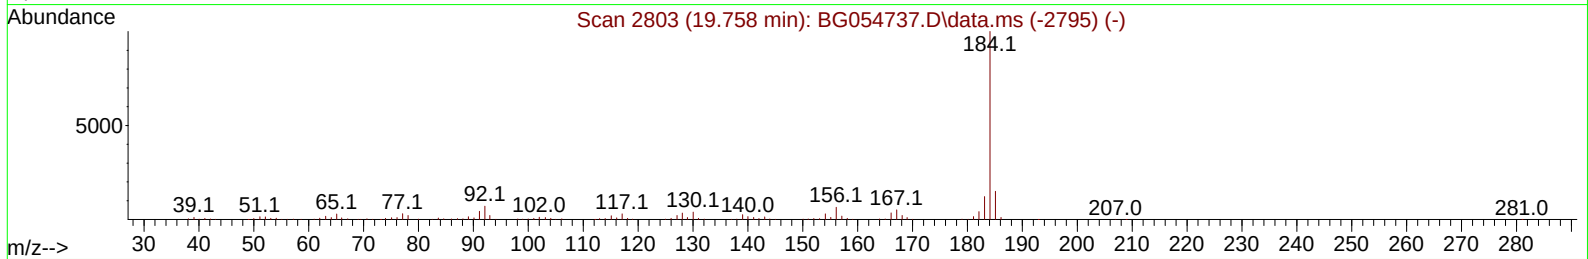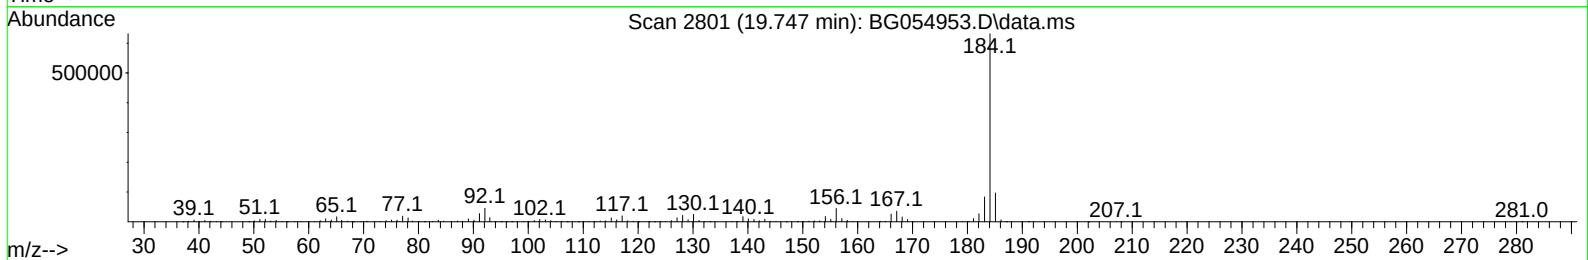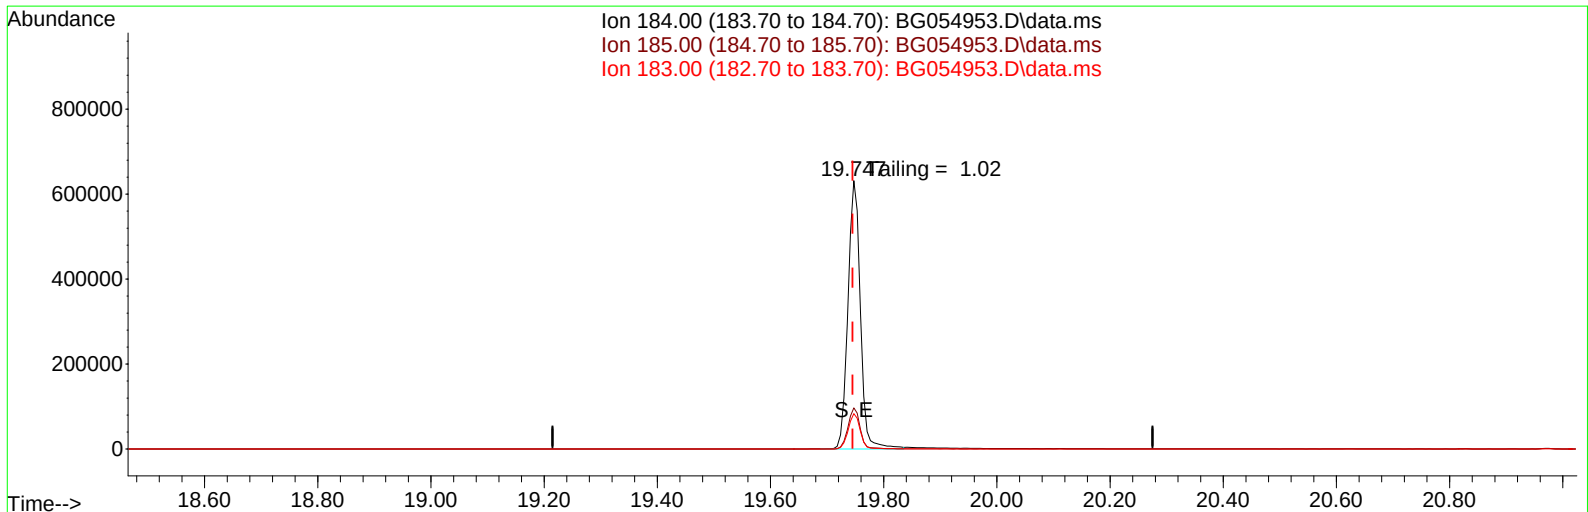

TIC: BG054953.D\data.ms

(77) Benzidine

19.747min (+ 0.003) 10312.03 ng

response 991271

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.31
183.00	12.30	13.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/15/2022	BNA_G	<u>BG054953.D</u>
Compound Name	Response	Retention Time
DDT	488285	20.969
DDD	6309	20.576
DDE	770	20.112
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7079	495364	1.43

Instrument :
BNA_G
ClientSampleId :
DFTPP