


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091525\
Data File : BG064368.D
Acq On : 15 Sep 2025 9:12
Operator : RC/JU
Sample : DFTPP458
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP458

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Sep 12 11:06:20 2025

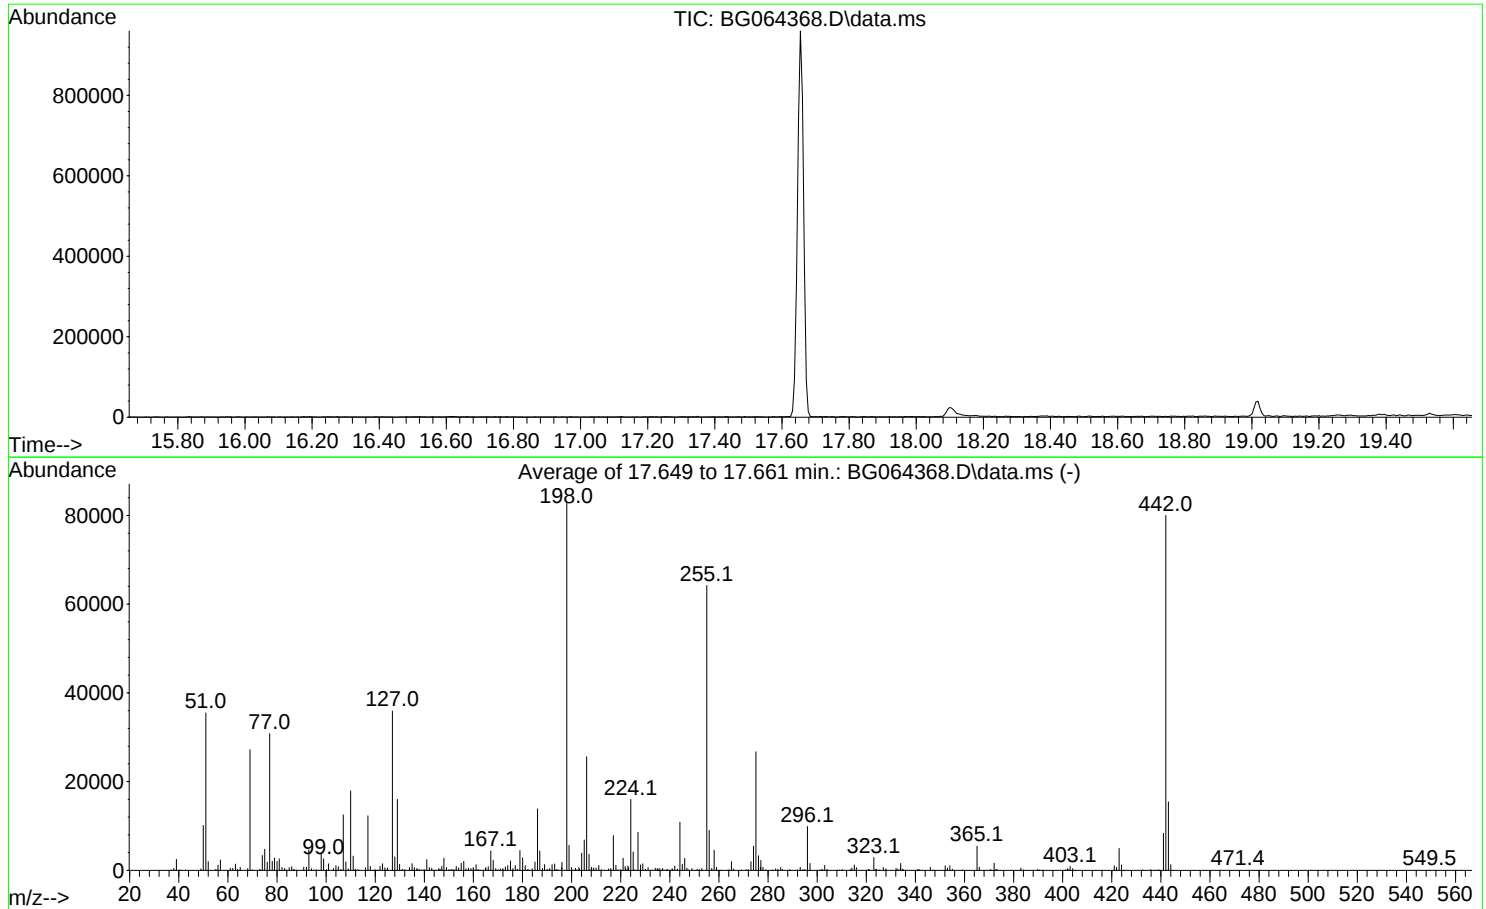

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	35485	PASS
68	69	0.00	2	1.4	384	PASS
69	198	0.00	100	32.8	27203	PASS
70	69	0.00	2	0.6	163	PASS
127	198	10	80	43.3	35923	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82909	PASS
199	198	5	9	6.8	5644	PASS
275	198	10	60	32.2	26733	PASS
365	198	1	100	6.6	5459	PASS
441	198	0.01	100	10.1	8385	PASS
442	198	50	100	96.5	79976	PASS
443	442	15	24	19.3	15441	PASS