


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091615\
Data File : BG018701.D
Acq On : 16 Sep 2015 8:59
Operator : UM/IZ
Sample : DFTPP47
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP47

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Title : SVOA CALIBRATION
Last Update : Thu Sep 17 02:24:24 2015

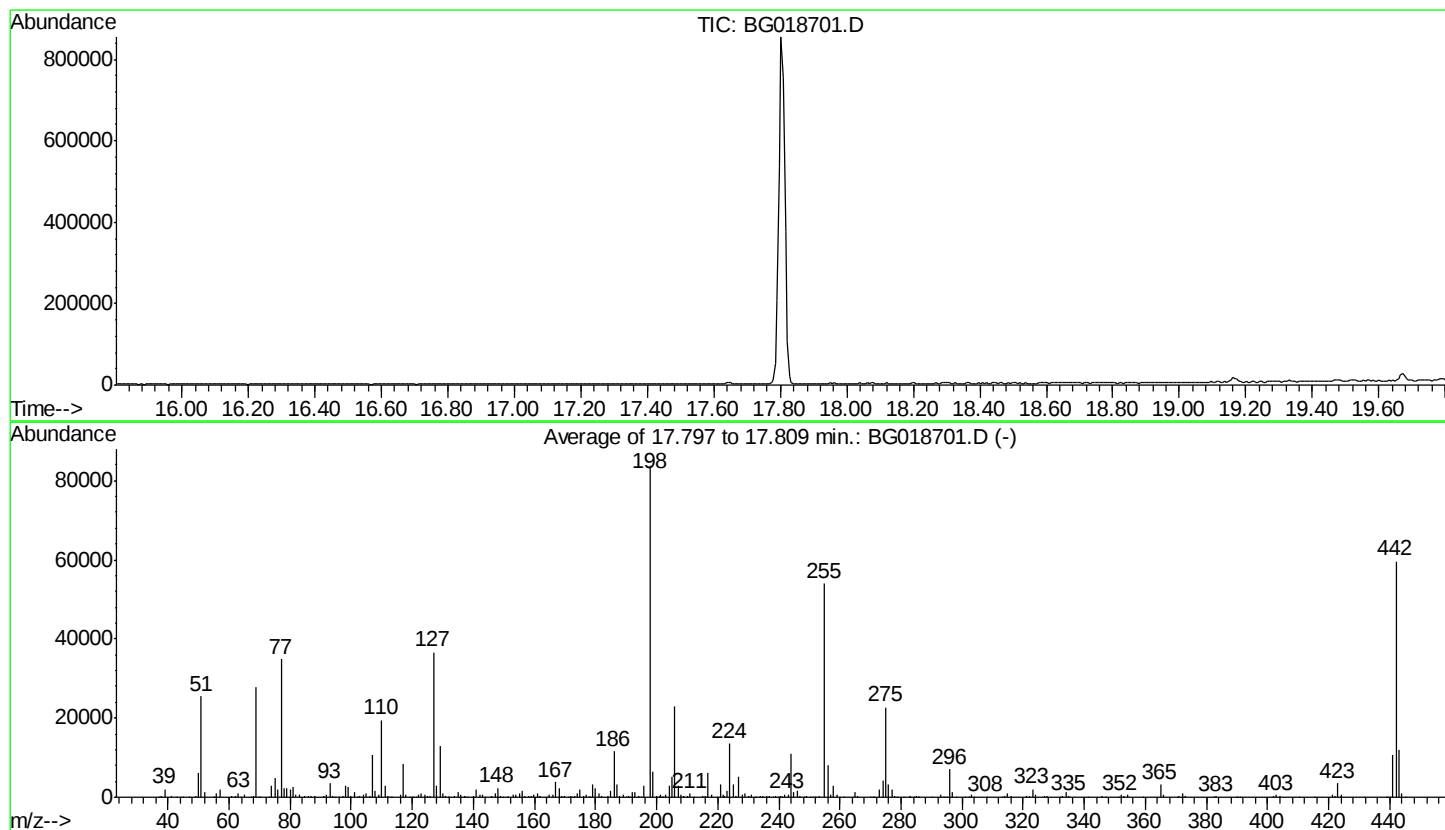

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	25472	PASS
68	69	0.00	2	0.7	192	PASS
69	198	0.00	100	33.0	27694	PASS
70	69	0.00	2	0.3	70	PASS
127	198	10	80	43.8	36693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83797	PASS
199	198	5	9	7.7	6443	PASS
275	198	10	60	27.0	22656	PASS
365	198	1	100	3.8	3153	PASS
441	442	0.01	24	17.7	10559	PASS
442	198	50	100	71.1	59600	PASS
443	442	15	24	19.9	11887	PASS

m/z	Abundance
38.00	298.0
39.00	1677.0
40.00	583.0
40.90	264.0
43.00	279.0
44.00	464.0
44.90	157.0
47.10	152.0
49.10	193.0
50.00	5656.0
51.00	23104.0
52.00	1253.0
54.90	214.0
56.00	620.0
56.90	1725.0
61.00	359.0
62.00	362.0
63.00	853.0
64.00	197.0
65.00	499.0
67.90	487.0
69.00	24400.0
72.90	190.0
74.00	2232.0
75.00	4669.0
76.00	1637.0
77.00	30688.0
78.00	1496.0
79.00	1872.0
80.00	1702.0
80.90	2443.0
81.90	476.0
83.00	746.0
84.90	479.0
85.90	616.0
86.90	284.0
91.00	435.0
92.00	479.0
92.90	3121.0
93.90	248.0
97.10	247.0
98.00	3063.0
98.90	2183.0
99.90	311.0
101.00	1215.0
103.00	293.0
103.90	1015.0
104.90	935.0
107.00	9411.0
107.90	1503.0
109.00	358.0
110.00	17112.0
111.00	2313.0
112.00	214.0
112.90	247.0
115.90	669.0
116.90	6347.0
118.00	678.0
120.00	188.0
121.90	746.0
122.90	879.0
124.00	556.0
124.90	418.0
125.80	432.0
127.00	29480.0
128.00	2210.0
129.00	11286.0
130.00	785.0
130.80	304.0
134.00	684.0
134.90	847.0
136.00	643.0
137.20	269.0
139.90	294.0
140.90	1296.0
141.90	556.0
143.00	549.0
144.00	234.0
145.80	185.0
146.10	177.0
147.00	907.0
147.90	1718.0
149.00	541.0
149.80	154.0
151.10	213.0
153.00	413.0
154.00	232.0
155.00	846.0
156.00	771.0
157.00	257.0
157.90	166.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

158.90	250.0
159.90	552.0
161.00	689.0
161.90	194.0
163.70	209.0
165.00	725.0
165.90	219.0
167.00	3414.0
167.90	2287.0
169.00	269.0
171.80	241.0
173.00	326.0
173.90	874.0
175.00	1084.0
176.00	381.0
176.90	583.0
177.80	177.0
178.90	2375.0
180.00	1780.0
181.00	1247.0
181.90	157.0
184.00	204.0
185.00	794.0
186.00	8932.0
186.90	2762.0
188.00	306.0
188.90	708.0
190.90	222.0
191.20	213.0
191.90	745.0
192.90	1282.0
194.10	331.0
196.00	1443.0
197.90	61944.0
198.90	5284.0
199.90	320.0
201.30	590.0
202.90	567.0
204.00	2261.0
205.00	4096.0
206.00	16182.0
207.00	2100.0
207.90	570.0
208.80	223.0
209.90	150.0
211.00	701.0
215.90	507.0
216.90	4916.0
217.90	378.0
219.80	206.0
220.90	2536.0
221.70	929.0
222.90	1094.0
224.00	9103.0
225.00	3144.0
226.10	299.0
227.00	3497.0
228.00	604.0
228.90	927.0
230.80	316.0
232.70	157.0
234.00	162.0
235.10	196.0
236.90	206.0
237.90	162.0
238.90	254.0
239.80	166.0
242.00	646.0
243.10	716.0
244.00	7315.0
245.00	840.0
245.90	1197.0
246.90	441.0
248.80	176.0
250.10	168.0
251.90	195.0
252.10	197.0
253.00	165.0
255.00	39528.0
256.00	5981.0
257.00	318.0
258.00	1730.0
259.00	470.0
261.00	151.0
263.90	157.0
265.00	1056.0
266.00	233.0
273.00	1482.0
274.00	2329.0
275.00	15650.0
276.00	2515.0
277.00	1237.0
277.90	218.0
279.00	182.0
281.00	217.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

282.90	367.0
284.90	401.0
293.00	465.0
293.90	251.0
294.90	204.0
296.00	4250.0
297.00	772.0
297.90	175.0
302.00	170.0
303.00	420.0
314.90	422.0
316.00	241.0
323.00	1063.0
324.00	404.0
326.90	156.0
327.90	303.0
334.00	700.0
346.00	311.0
352.00	254.0
353.00	284.0
354.00	384.0
365.00	1700.0
366.00	303.0
371.00	151.0
372.10	812.0
373.00	196.0
389.60	168.0
401.80	316.0
402.90	276.0
415.20	178.0
421.00	311.0
422.00	264.0
423.00	2312.0
423.90	347.0
441.00	5799.0
442.00	35208.0
443.00	6610.0
443.90	522.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

m/z	Abundance
36.80	211.0
37.60	221.0
38.00	480.0
39.00	2872.0
39.90	908.0
43.00	166.0
44.00	608.0
49.00	458.0
50.00	7456.0
51.00	31152.0
52.00	1349.0
54.90	185.0
55.90	1067.0
57.00	2723.0
60.90	267.0
62.00	484.0
63.00	1767.0
63.90	170.0
65.00	417.0
67.00	160.0
68.10	578.0
69.00	34264.0
72.90	289.0
74.00	4286.0
75.00	6374.0
76.00	2374.0
77.00	41928.0
78.00	2572.0
79.00	2821.0
79.90	2325.0
80.90	2651.0
81.90	686.0
83.00	929.0
84.90	522.0
86.00	743.0
87.00	478.0
87.90	266.0
91.00	606.0
91.90	683.0
92.90	4223.0
94.00	517.0
94.90	281.0
95.90	309.0
97.10	360.0
98.00	3340.0
98.90	3061.0
99.80	188.0
101.00	1402.0
102.90	654.0
103.90	887.0
105.00	1243.0
106.00	307.0
107.00	11874.0
107.90	1796.0
108.80	602.0
110.00	22568.0
111.00	3451.0
111.90	402.0
113.10	261.0
115.90	736.0
117.00	10939.0
117.90	1014.0
119.00	267.0
120.20	156.0
121.00	229.0
121.90	548.0
123.00	1538.0
123.90	506.0
124.90	323.0
127.00	44024.0
127.90	3205.0
128.90	15432.0
129.90	1239.0
130.90	427.0
131.80	153.0
133.90	507.0
135.00	1697.0
136.00	477.0
136.90	769.0
140.00	189.0
140.90	2537.0
142.00	843.0
143.00	686.0
144.00	223.0
146.00	260.0
147.00	1166.0
148.00	2791.0
149.00	501.0
149.80	219.0
151.50	170.0
152.90	983.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

153.90	561.0
155.00	1527.0
156.00	2191.0
156.90	360.0
158.00	364.0
158.90	390.0
159.90	749.0
161.00	1211.0
162.00	408.0
163.80	184.0
164.90	814.0
165.90	1019.0
167.00	4795.0
167.90	2866.0
168.80	373.0
169.80	289.0
171.80	220.0
172.40	190.0
173.00	438.0
174.00	927.0
175.00	2217.0
176.00	625.0
177.00	755.0
178.00	356.0
178.90	4062.0
179.90	2841.0
181.00	1286.0
182.00	221.0
183.90	347.0
185.00	2384.0
186.00	13396.0
187.00	4102.0
187.90	224.0
189.00	525.0
189.80	159.0
190.90	693.0
192.00	1326.0
193.00	1483.0
194.10	518.0
195.00	577.0
196.00	3199.0
197.90	100392.0
198.90	6957.0
199.90	582.0
200.60	245.0
201.40	486.0
201.70	429.0
203.00	527.0
204.00	3547.0
205.00	6580.0
206.00	28448.0
207.00	4223.0
208.00	941.0
209.00	533.0
209.90	507.0
210.80	961.0
212.10	201.0
215.00	471.0
215.90	692.0
216.90	7999.0
218.00	1209.0
221.00	3935.0
222.00	815.0
223.00	1675.0
224.00	16656.0
225.00	3260.0
225.90	566.0
226.90	6315.0
228.00	803.0
229.00	1235.0
230.00	303.0
230.90	677.0
232.10	161.0
234.00	651.0
234.90	480.0
235.90	300.0
236.90	642.0
239.00	312.0
239.80	223.0
240.80	572.0
242.00	760.0
243.00	767.0
244.00	13681.0
245.00	1674.0
246.00	2159.0
247.00	401.0
248.10	198.0
249.00	520.0
251.80	163.0
253.00	426.0
255.00	64128.0
256.00	9845.0
256.90	1095.0
257.90	3420.0
258.90	656.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

259.80	303.0
264.90	1391.0
265.90	620.0
270.10	237.0
270.80	332.0
272.90	1634.0
273.90	4957.0
275.00	26496.0
276.00	3638.0
277.00	2484.0
277.90	481.0
278.80	156.0
283.10	314.0
284.00	272.0
284.90	252.0
285.50	157.0
290.20	153.0
293.00	511.0
294.20	175.0
295.90	8923.0
296.90	887.0
301.10	195.0
302.00	191.0
303.00	878.0
304.10	187.0
314.00	416.0
314.90	1085.0
316.00	492.0
321.00	395.0
321.80	186.0
323.00	2519.0
323.90	668.0
326.90	635.0
327.90	378.0
331.90	205.0
332.90	246.0
334.00	1759.0
335.00	488.0
345.90	613.0
347.00	158.0
351.10	157.0
351.90	799.0
353.00	326.0
354.00	988.0
365.00	3762.0
365.90	870.0
370.50	174.0
371.00	222.0
371.90	1199.0
372.90	393.0
383.10	316.0
401.90	310.0
403.00	609.0
404.00	251.0
421.00	753.0
422.00	607.0
423.00	3536.0
424.10	774.0
431.50	204.0
440.10	167.0
441.10	12549.0
442.00	66584.0
443.10	14417.0
444.00	1433.0
444.90	162.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

m/z	Abundance
39.00	1795.0
40.00	561.0
41.00	315.0
44.00	605.0
48.90	371.0
50.00	5310.0
51.00	22160.0
52.00	955.0
55.10	231.0
56.00	802.0
57.00	1640.0
58.00	283.0
60.90	312.0
62.00	296.0
63.00	803.0
65.00	581.0
68.90	25120.0
69.70	194.0
69.90	211.0
72.80	381.0
74.00	2318.0
75.00	3926.0
76.00	1826.0
77.00	31936.0
78.00	2330.0
79.00	1656.0
80.00	1522.0
81.00	2247.0
81.90	594.0
83.00	386.0
83.90	199.0
85.00	323.0
85.90	589.0
86.90	239.0
87.90	256.0
91.00	854.0
92.00	467.0
93.00	3311.0
94.00	305.0
96.00	171.0
98.00	2626.0
99.00	2290.0
100.00	175.0
101.00	1513.0
101.80	155.0
102.90	487.0
104.00	469.0
105.00	989.0
105.80	260.0
106.90	11189.0
108.00	1783.0
109.00	586.0
109.90	18992.0
111.00	3160.0
111.90	448.0
116.00	710.0
116.90	8109.0
117.90	390.0
121.80	655.0
123.00	896.0
123.90	558.0
124.90	344.0
125.70	169.0
127.00	36576.0
128.00	3294.0
128.90	12218.0
129.90	818.0
131.00	206.0
132.00	251.0
133.90	604.0
135.00	1369.0
135.90	548.0
137.00	475.0
137.80	226.0
139.90	348.0
141.00	1624.0
141.90	668.0
142.90	324.0
146.10	297.0
147.00	775.0
147.90	2548.0
149.00	314.0
152.90	826.0
153.90	1036.0
154.90	750.0
155.90	1460.0
156.90	284.0
158.00	338.0
158.90	397.0
159.90	1046.0
161.00	1002.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

161.60	316.0
162.00	220.0
164.90	757.0
166.00	741.0
167.00	3550.0
168.00	1971.0
169.00	395.0
169.90	263.0
171.00	150.0
171.90	545.0
173.00	401.0
173.90	1240.0
175.00	2098.0
176.00	388.0
176.90	415.0
177.80	276.0
178.90	3377.0
180.00	2114.0
181.00	869.0
182.00	243.0
183.90	249.0
184.90	1640.0
186.00	12280.0
186.90	3269.0
188.00	368.0
188.90	790.0
191.10	262.0
191.90	1468.0
193.00	820.0
193.90	515.0
194.80	254.0
195.90	3748.0
197.90	89056.0
198.90	7089.0
199.90	457.0
200.90	160.0
201.40	424.0
202.10	165.0
202.90	705.0
204.00	3137.0
205.00	4698.0
206.00	24696.0
207.00	3341.0
207.90	788.0
208.90	334.0
210.20	296.0
211.00	898.0
212.00	238.0
215.00	203.0
216.20	489.0
216.90	5947.0
217.90	865.0
219.80	183.0
221.00	2801.0
221.70	1018.0
223.00	2292.0
224.00	14572.0
225.00	2966.0
226.00	399.0
226.90	5977.0
227.90	1051.0
229.00	1168.0
229.90	253.0
230.90	829.0
232.00	164.0
234.00	517.0
234.80	579.0
236.00	258.0
236.90	594.0
239.00	245.0
240.00	249.0
241.00	309.0
242.00	609.0
243.00	767.0
244.00	12168.0
245.00	1591.0
245.90	2005.0
247.00	431.0
248.10	257.0
248.90	359.0
250.00	242.0
250.90	174.0
253.00	243.0
255.00	58392.0
256.00	8884.0
256.90	732.0
257.90	3519.0
259.00	780.0
264.00	176.0
265.00	1835.0
266.00	267.0
271.10	209.0
273.00	2509.0
274.00	5239.0
275.00	25824.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

276.00	3805.0
276.90	2564.0
277.80	180.0
278.90	165.0
283.00	416.0
285.00	388.0
285.90	241.0
293.00	918.0
294.10	175.0
296.00	7827.0
296.90	1855.0
297.90	210.0
302.20	288.0
303.00	960.0
304.00	198.0
307.90	191.0
313.00	160.0
313.90	362.0
315.00	1049.0
316.00	638.0
321.00	340.0
322.00	285.0
323.00	2250.0
323.90	470.0
326.90	465.0
328.00	461.0
333.00	353.0
334.10	1779.0
335.00	621.0
341.00	222.0
345.90	370.0
352.00	681.0
353.00	477.0
353.90	624.0
359.30	157.0
365.00	3997.0
365.90	657.0
371.00	262.0
372.00	927.0
373.00	309.0
382.40	162.0
383.10	415.0
390.10	181.0
391.00	165.0
402.00	474.0
402.90	1054.0
403.80	252.0
404.10	300.0
410.10	152.0
421.10	428.0
421.90	462.0
423.00	4440.0
424.00	1035.0
438.70	185.0
439.30	190.0
441.00	13329.0
442.00	77008.0
443.00	14635.0
444.00	1291.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47

m/z	Abundance
39.90	723.0
42.30	154.0
44.00	446.0
58.00	173.0
59.10	150.0
69.10	234.0
73.00	192.0
83.80	191.0
85.80	198.0
91.00	224.0
134.10	197.0
149.10	209.0
167.00	180.0
194.80	212.0
207.00	393.0

Instrument :
BNA_G
ClientSampleId :
DFTPP47