
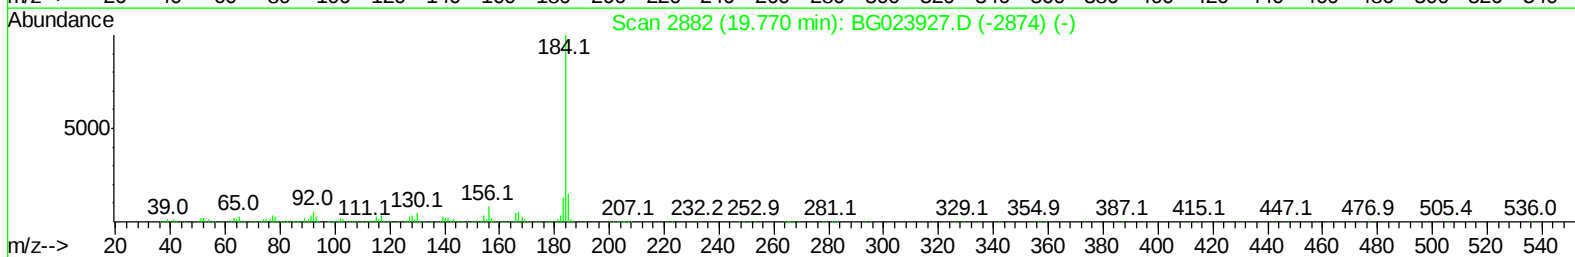
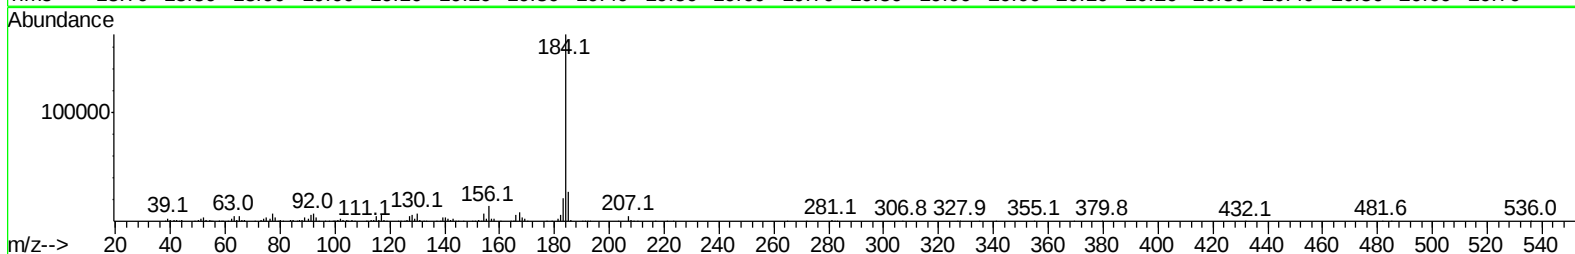


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG023992.D
Acq On : 16 Sep 2016 14:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:53:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 04:50:01 2016
Response via : Initial Calibration

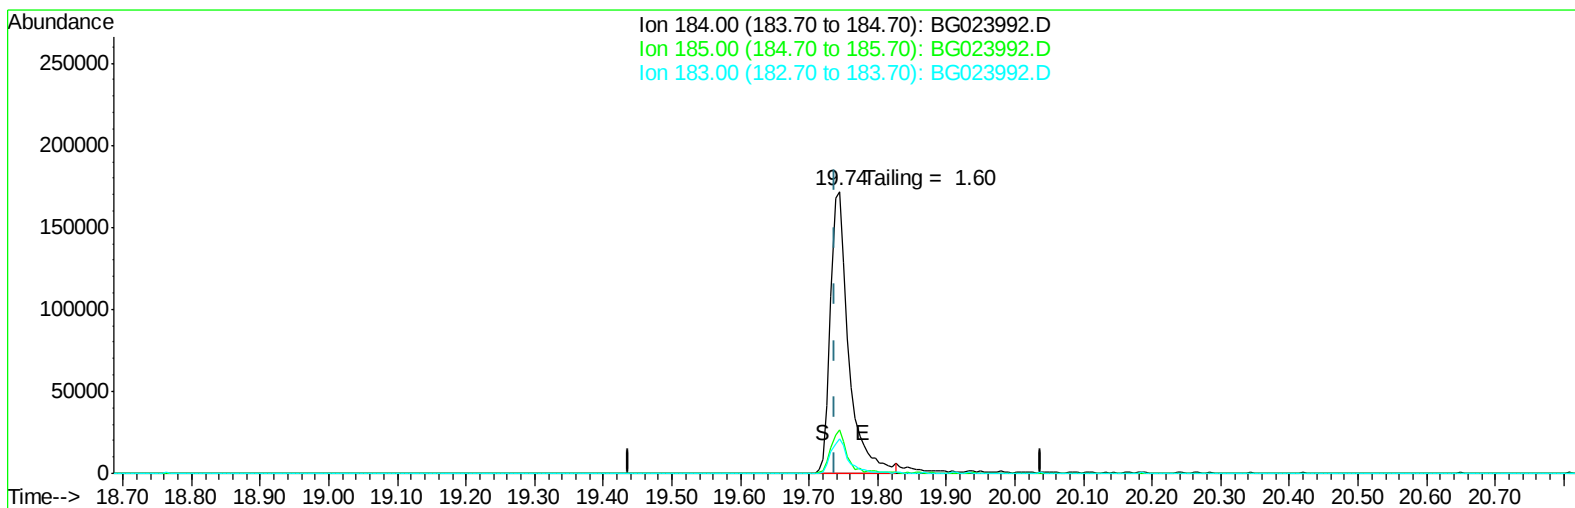

TIC: BG023992.D

(76) Benzidine




19.744min (+0.006) 119033.86ng

response 313308

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.52
183.00	13.40	12.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG023992.D
Acq On : 16 Sep 2016 14:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:53:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 04:50:01 2016
Response via : Initial Calibration

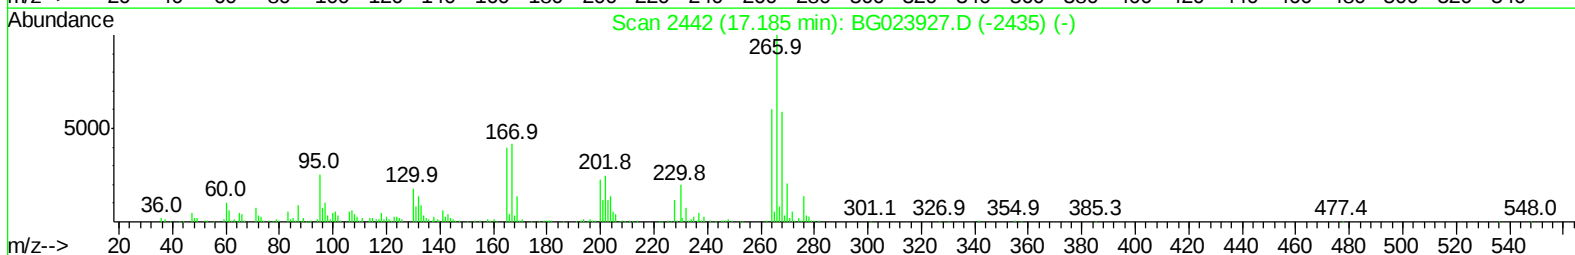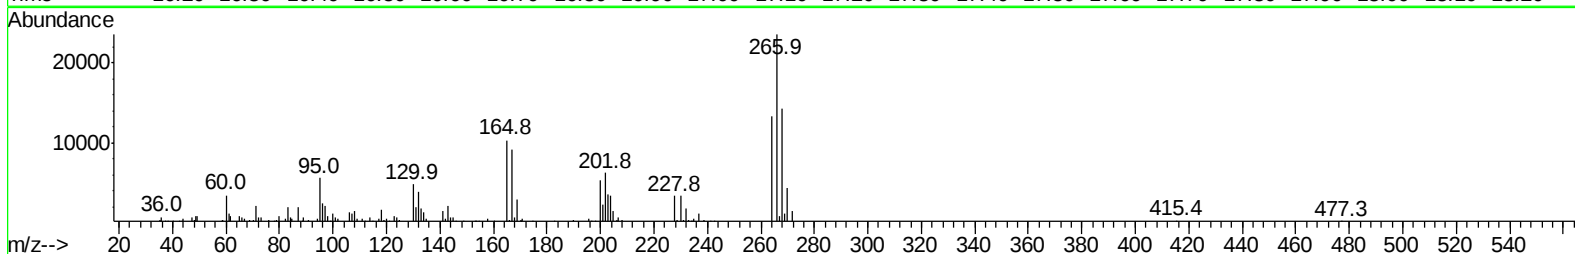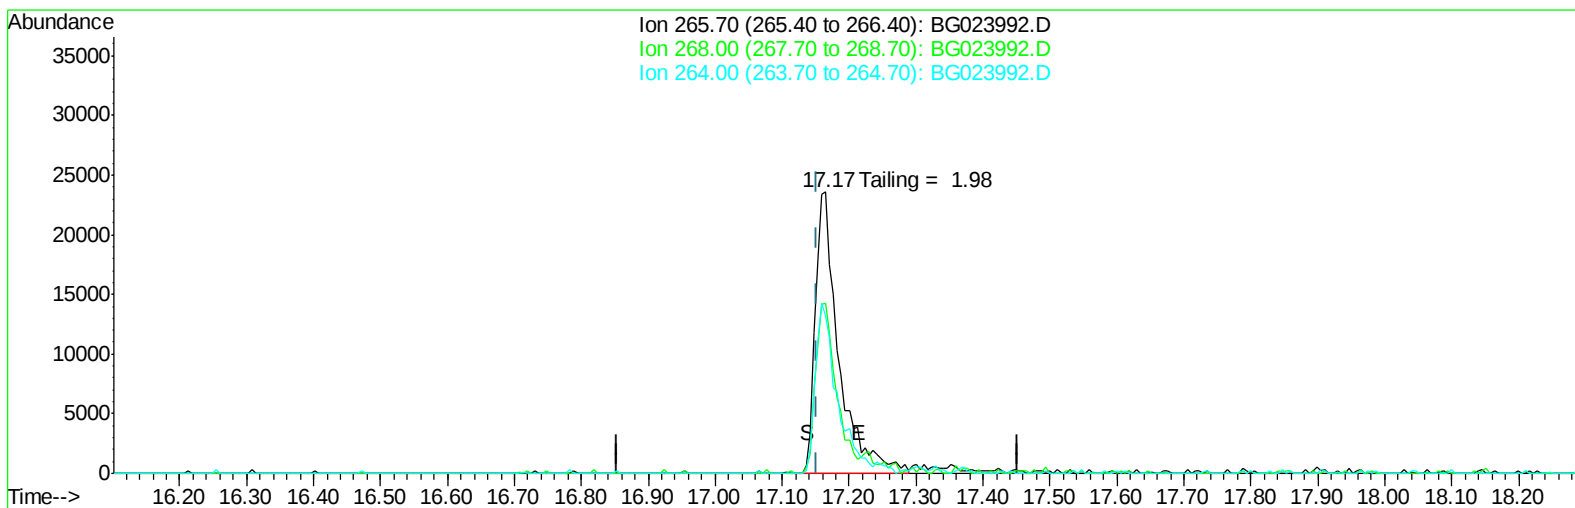

TIC: BG023992.D

(69) Pentachlorophenol (C)

17.165min (+0.012) 80924.62ng

response 58262

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	60.40
264.00	63.20	56.14
0.00	0.00	0.00