
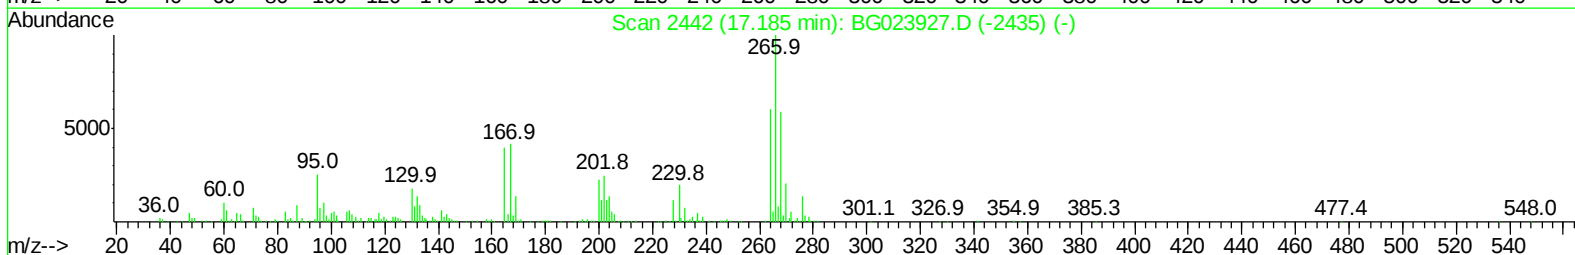
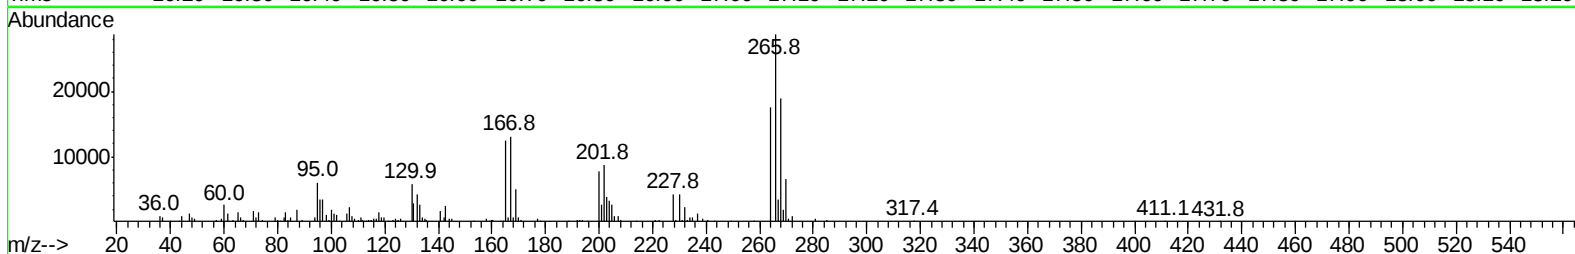


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG024009.D
Acq On : 17 Sep 2016 1:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:54:49 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 04:50:01 2016
Response via : Initial Calibration

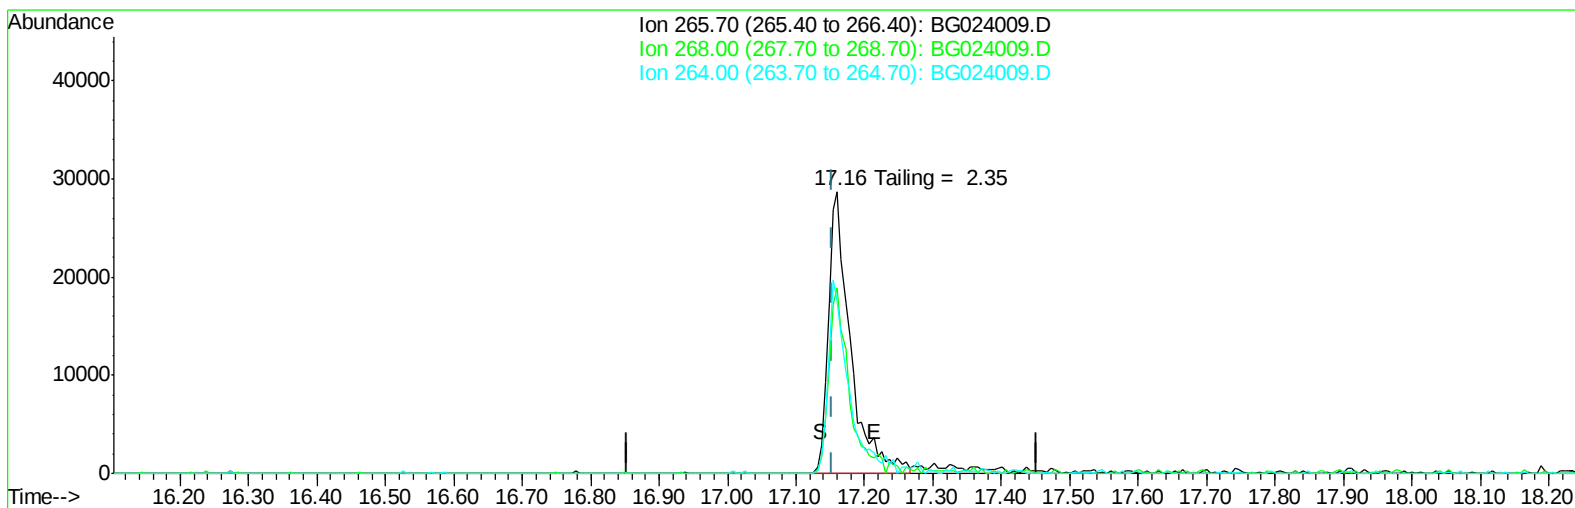

TIC: BG024009.D

(69) Pentachlorophenol (C)




17.160min (+0.007) 78543.39ng

response 62500

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	66.13
264.00	63.20	61.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG024009.D
Acq On : 17 Sep 2016 1:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:54:49 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 04:50:01 2016
Response via : Initial Calibration

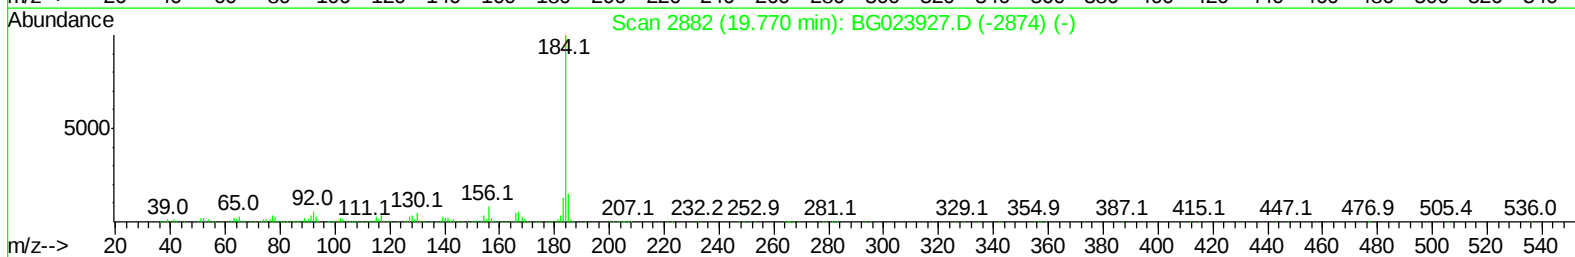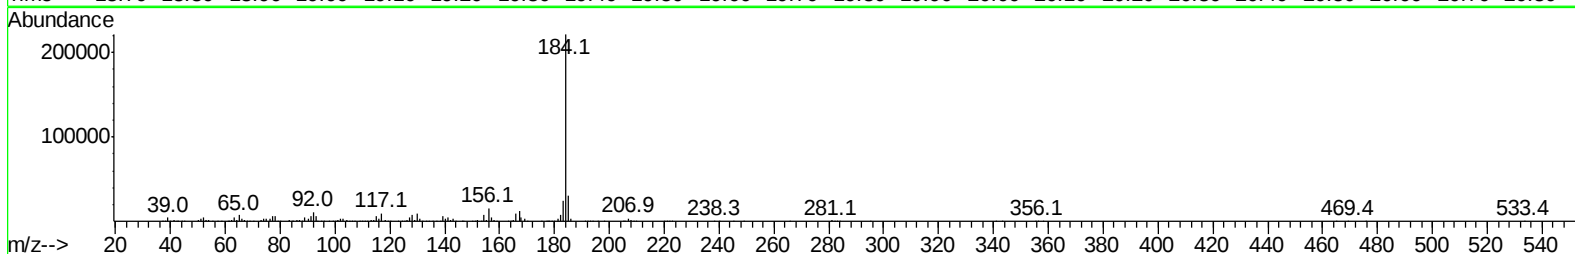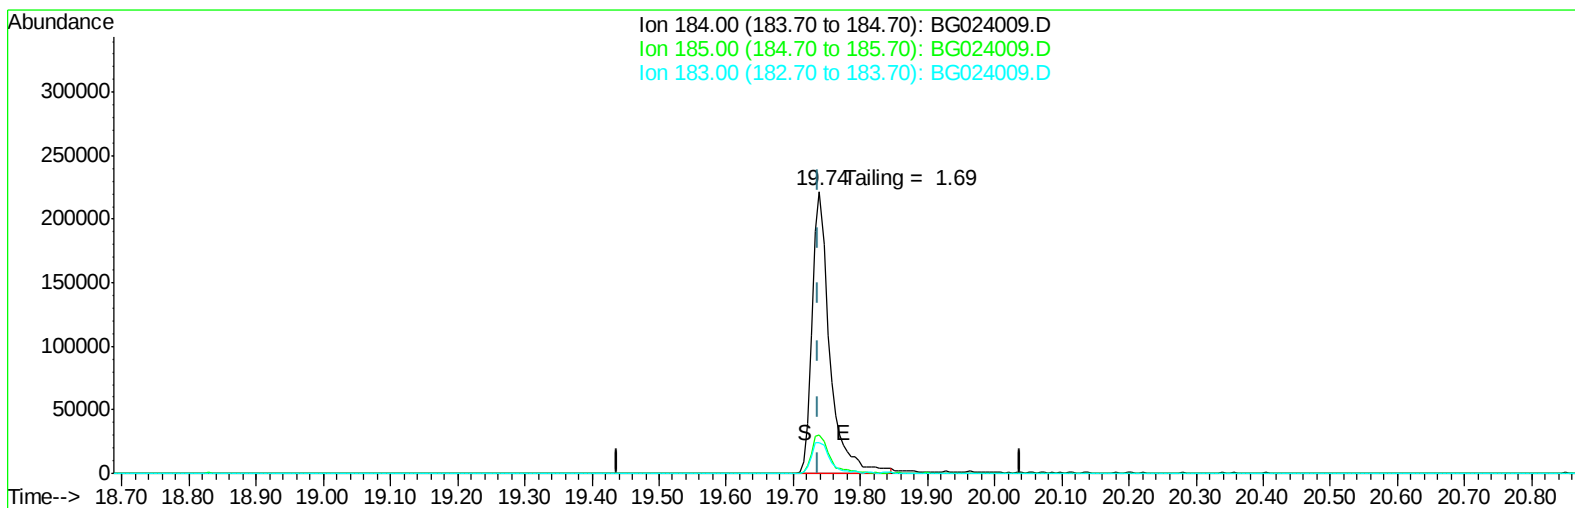

TIC: BG024009.D

(76) Benzidine

19.739min (+0.001) 180976.69ng

response 397890

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.79
183.00	13.40	11.14
0.00	0.00	0.00