

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
 Data File : BG024001.D
 Acq On : 16 Sep 2016 19:59
 Operator : UM/SJ
 Sample : H4802-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BRC001-AT01-AQ002-01

Quant Time: Sep 17 00:39:52 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 17 00:17:46 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	49252	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	219563	20.00	ng	0.00
38) Acenaphthene-d10	14.73	164	198064	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	487933	20.00	ng	0.00
75) Chrysene-d12	21.80	240	491362	20.00	ng	0.00
86) Perylene-d12	25.15	264	493874	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	156725	55.87	ng	0.00
7) Phenol-d6	7.23	99	133462	30.91	ng	0.00
23) Nitrobenzene-d5	9.24	82	469549	95.47	ng	0.00
41) 2,4,6-Tribromophenol	16.23	330	418676	117.33	ng	0.00
44) 2-Fluorobiphenyl	13.34	172	1005782	72.81	ng	0.00
78) Terphenyl-d14	20.10	244	1397202	64.76	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.18	163	130042	7.66	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG024001.D
Acq On : 16 Sep 2016 19:59
Operator : UM/SJ
Sample : H4802-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BRC001-AT01-AQ002-01

Quant Time: Sep 17 00:39:52 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 00:17:46 2016
Response via : Initial Calibration

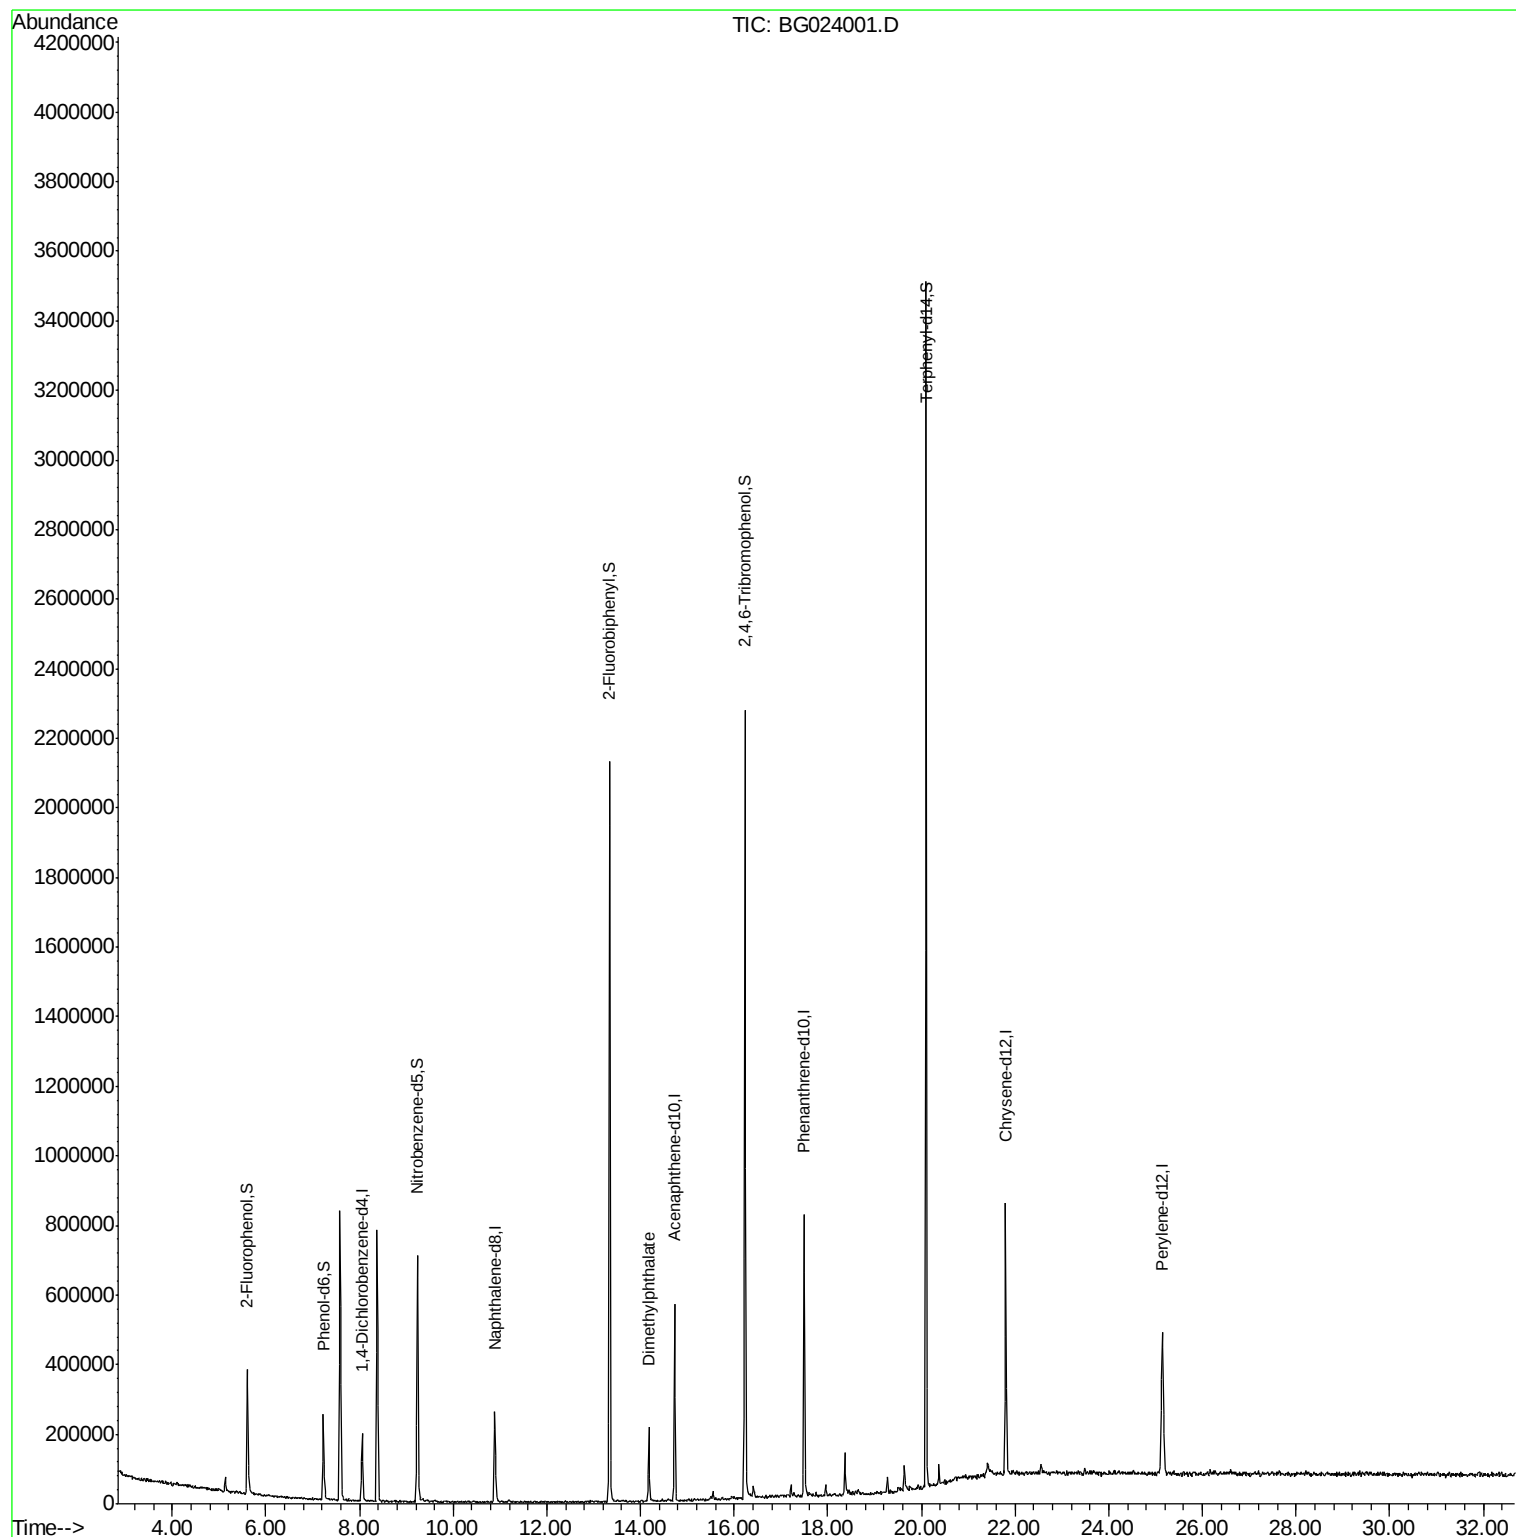

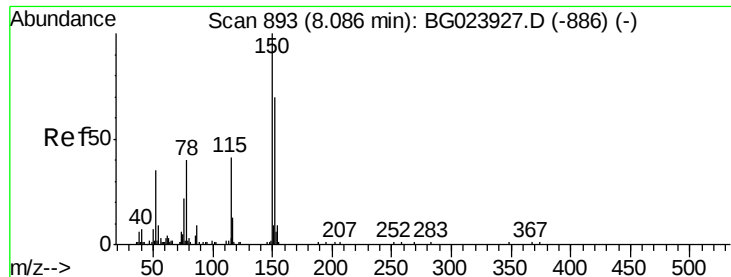

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.05 min Scan# 888

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59

Instrument :

BNA_G

ClientSampleId :

BRC001-AT01-AQ002-01


Tot Ion:152 Resp: 49252

Ion Ratio Lower Upper

152 100

150 148.5 144.7 217.1




115 78.5 64.0 96.0

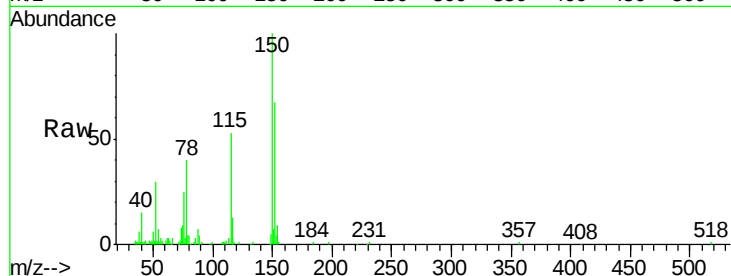

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

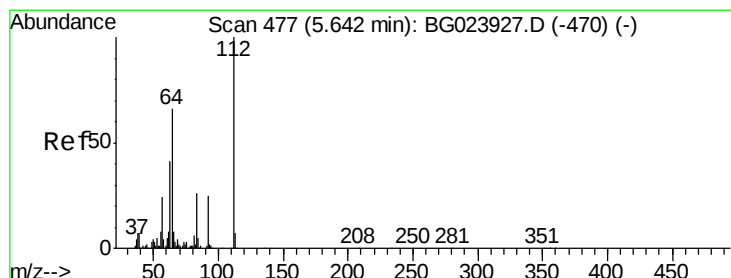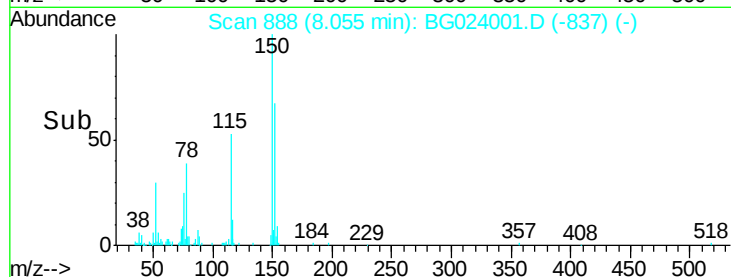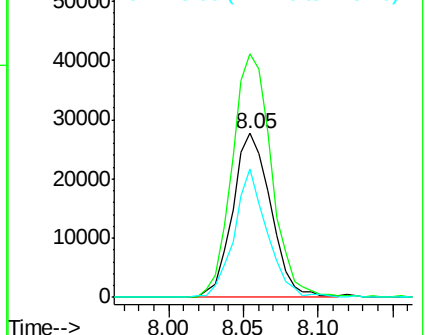

#5

2-Fluorophenol

Concen: 55.87 ng

RT: 5.60 min Scan# 471

Delta R.T. 0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59


Tgt Ion:112 Resp: 156725

Ion Ratio Lower Upper

112 100

64 69.9 59.0 88.4



63 44.8 37.8 56.8

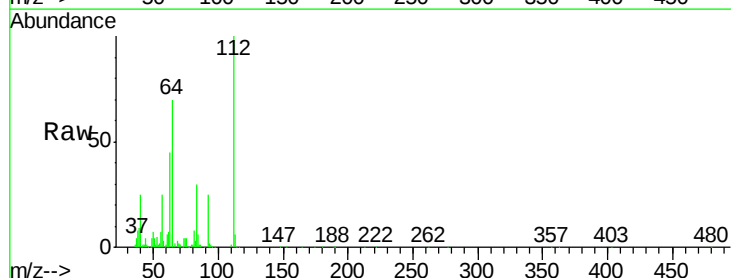


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

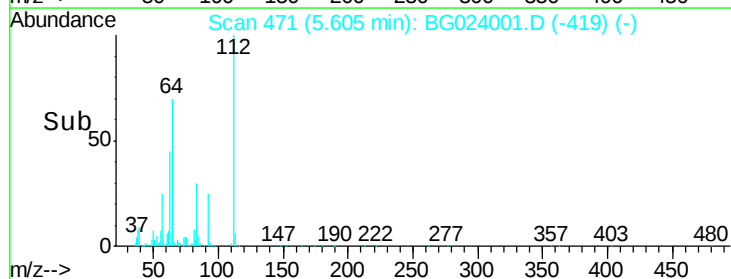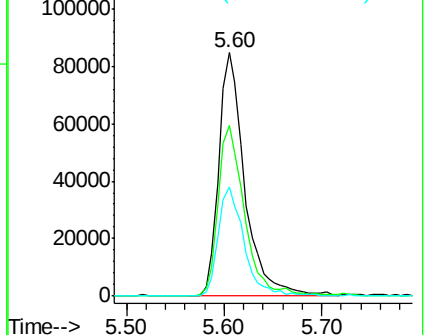

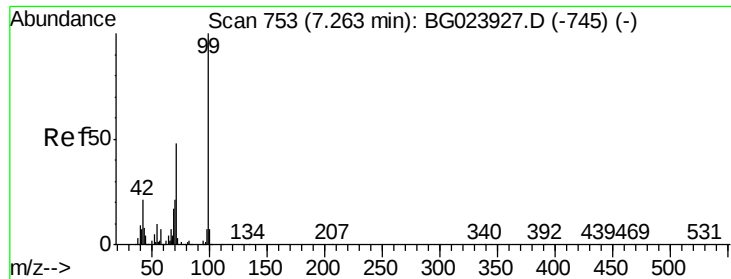

#7

Phenol-d6

Concen: 30.91 ng

RT: 7.23 min Scan# 747

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59

Instrument :

BNA_G

ClientSampleId :

BRC001-AT01-AQ002-01


Tot Ion: 99 Resp: 133462

Ion Ratio Lower Upper




99 100

42 25.1 17.8 26.6

71 52.5 41.5 62.3

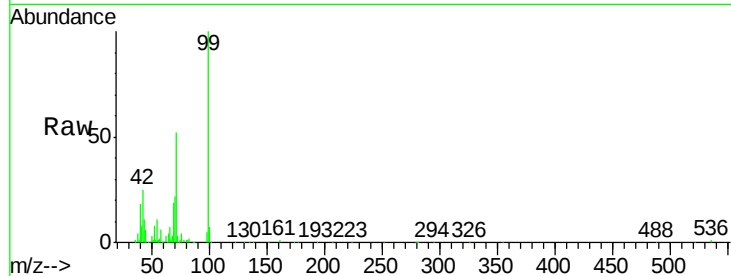

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

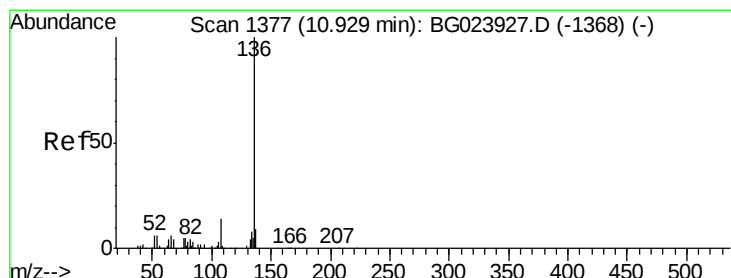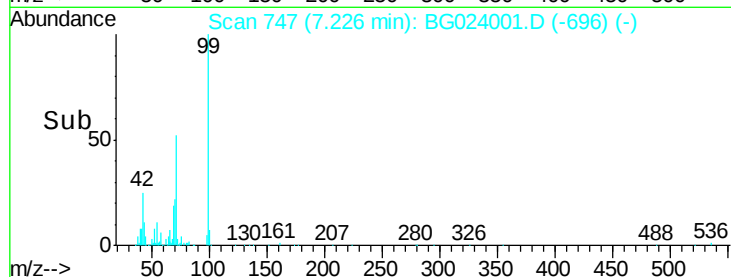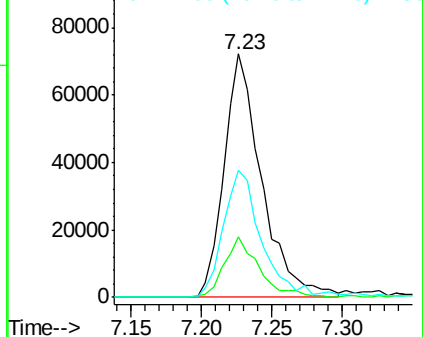

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.89 min Scan# 1370

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59

Tgt Ion: 136 Resp: 219563


Ion Ratio Lower Upper

136 100



137 10.2 9.6 14.4


54 8.9 7.3 10.9

68 5.0 5.3 7.9#

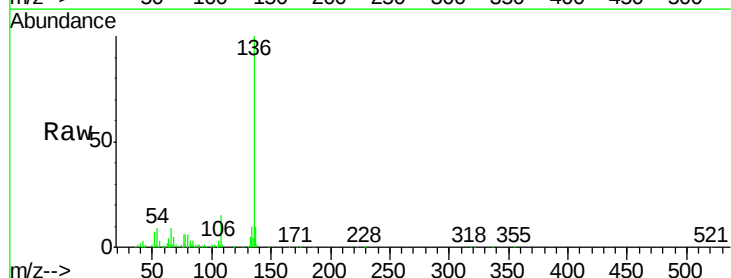

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



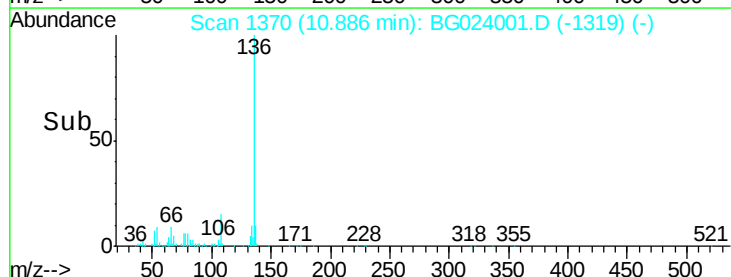
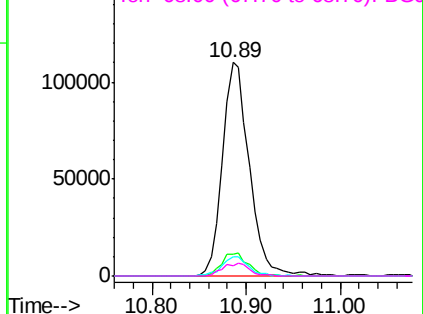


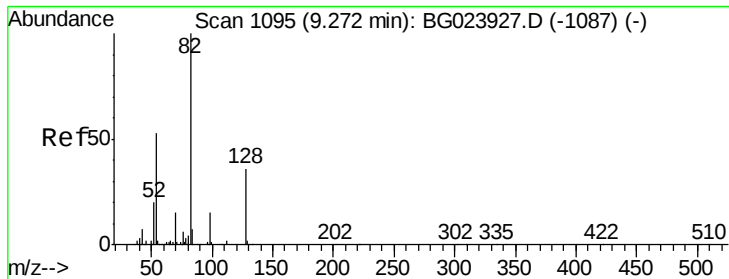

#23
Nitrobenzene-d5
Concen: 95.47 ng
RT: 9.24 min Scan# 1089
Delta R.T. -0.00 min
Lab File: BG024001.D
Acq: 16 Sep 2016 19:59




Instrument :
BNA_G
ClientSampleId :
BRC001-AT01-AQ002-01


Tot Ion	82	Resp	469549
Ion Ratio	Lower	Upper	
82	100		
128	31.6	24.4	36.6
54	51.7	41.4	62.0

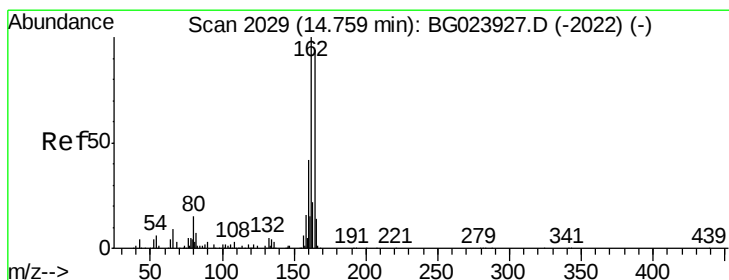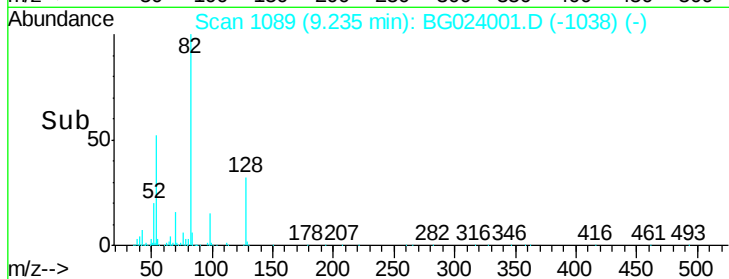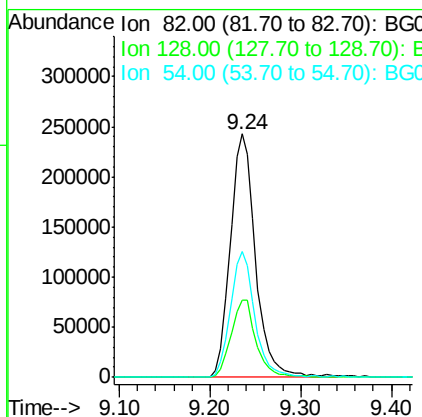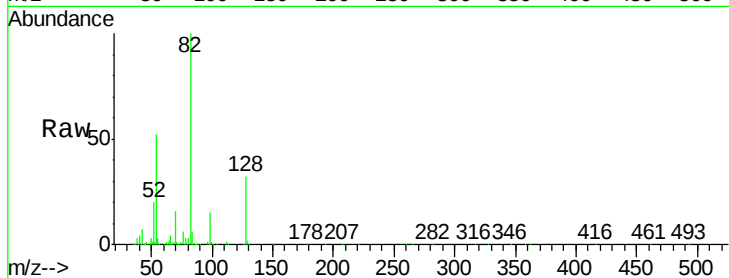

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.73 min Scan# 2024
Delta R.T. -0.00 min
Lab File: BG024001.D
Acq: 16 Sep 2016 19:59

Tgt Ion	164	Resp	198064
Ion Ratio	Lower	Upper	
164	100		
162	106.7	87.7	131.5
160	45.0	37.2	55.8


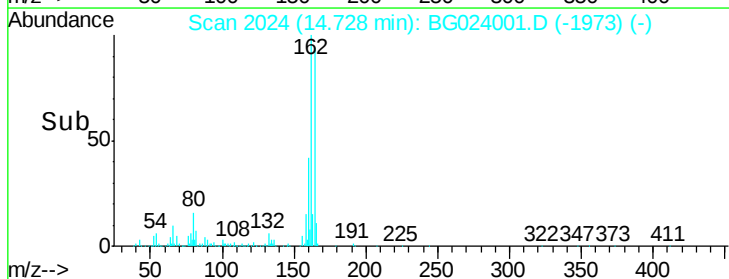
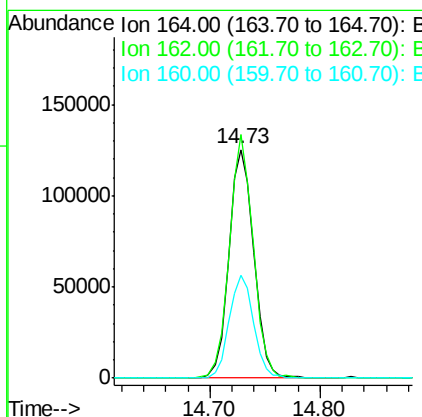
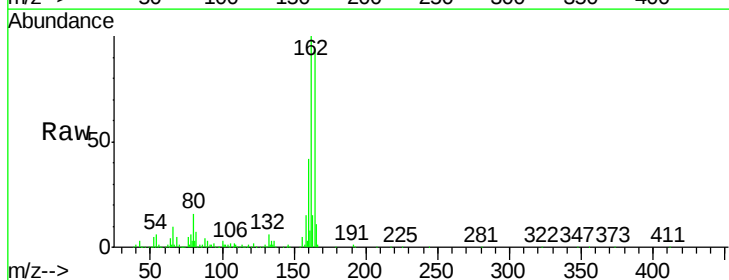


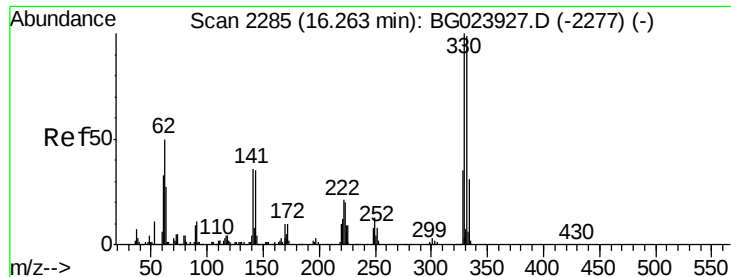

#41
 2,4,6-Tribromophenol
 Concen: 117.33 ng
 RT: 16.23 min Scan# 2280
 Delta R.T. -0.00 min
 Lab File: BG024001.D
 Acq: 16 Sep 2016 19:59




Instrument :
 BNA_G
 ClientSampleId :
 BRC001-AT01-AQ002-01


Tot Ion:330 Resp: 418676
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.4 116.2
 141 39.8 31.7 47.5

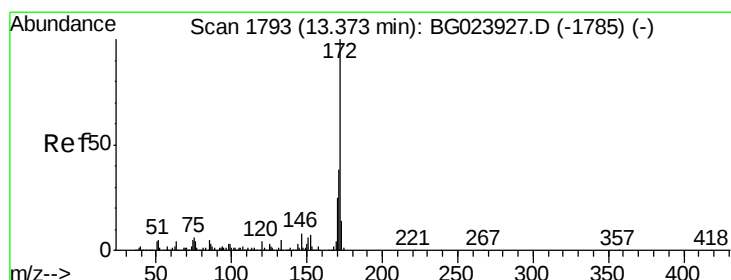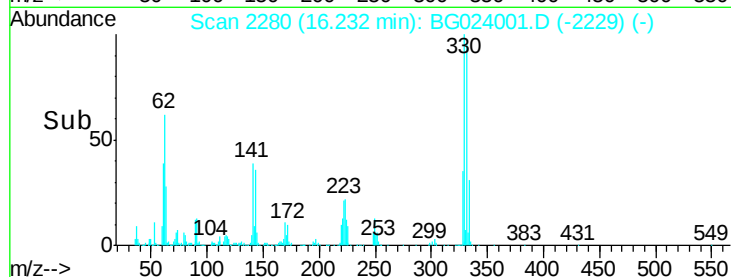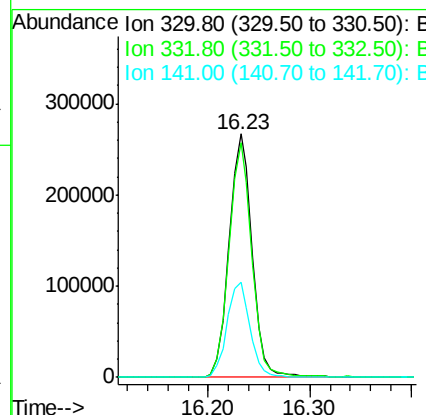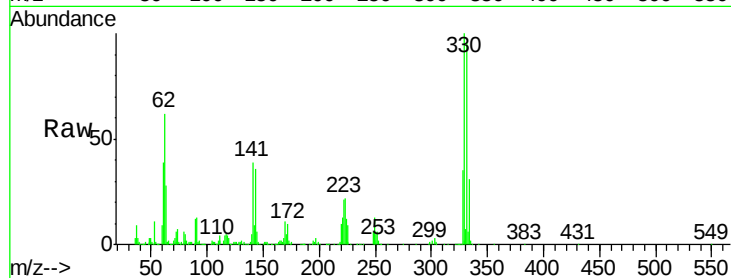

#44
 2-Fluorobiphenyl
 Concen: 72.81 ng
 RT: 13.34 min Scan# 1788
 Delta R.T. -0.00 min
 Lab File: BG024001.D
 Acq: 16 Sep 2016 19:59

Tgt Ion:172 Resp: 1005782
 Ion Ratio Lower Upper
 172 100
 171 37.8 31.6 47.4
 170 25.3 21.3 31.9

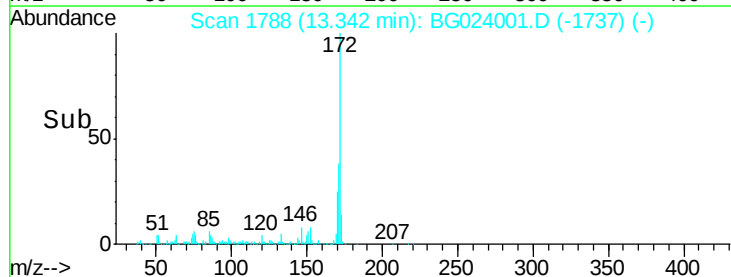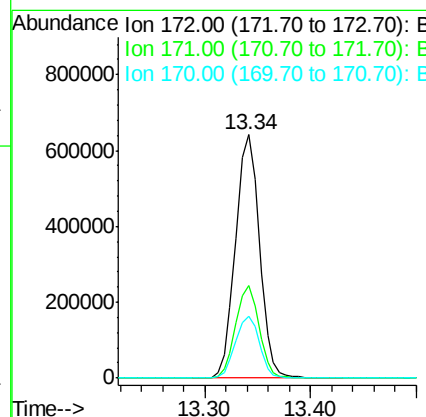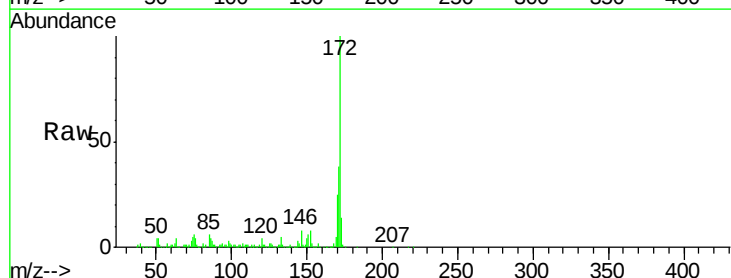

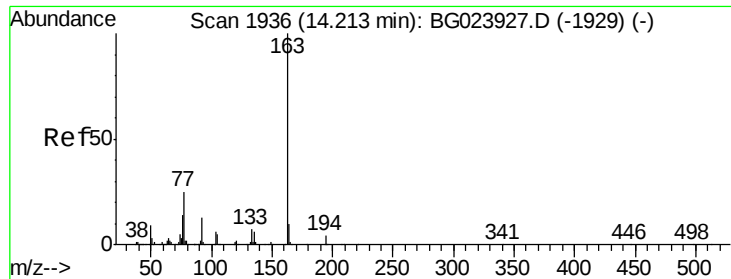

#49

Dimethylphthalate

Concen: 7.66 ng

RT: 14.18 min Scan# 1930

Delta R.T. -0.01 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59

Instrument :

BNA_G

ClientSampleId :

BRC001-AT01-AQ002-01


Tot Ion:163 Resp: 130042

Ion Ratio Lower Upper

163 100

194 2.8 3.6 5.4#




164 10.8 8.1 12.1

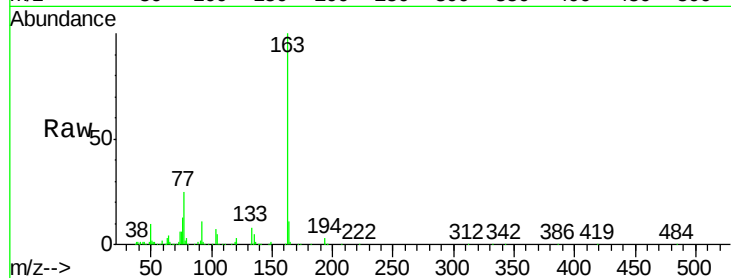

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

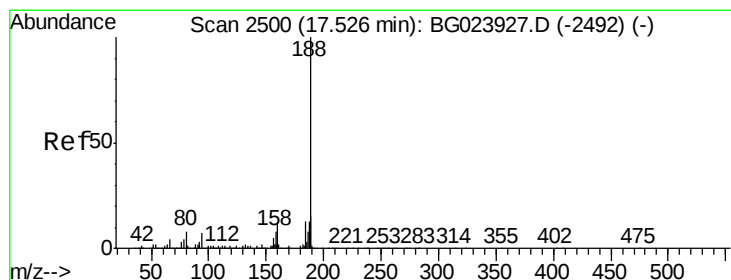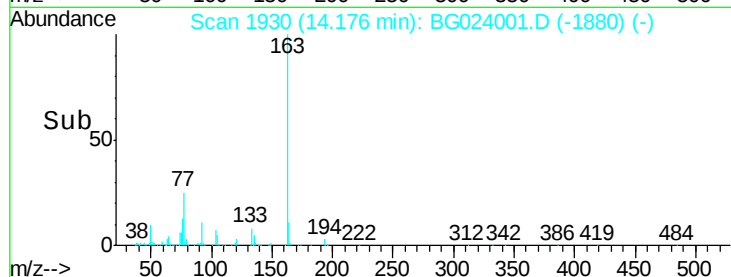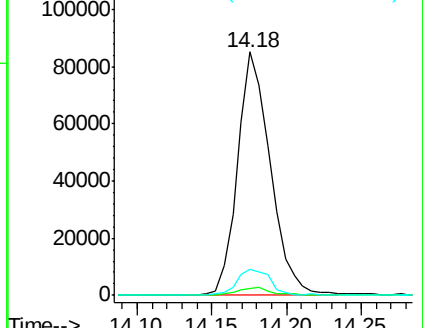

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.49 min Scan# 2495

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59


Tgt Ion:188 Resp: 487933

Ion Ratio Lower Upper

188 100

94 7.0 5.2 7.8



80 8.7 7.2 10.8

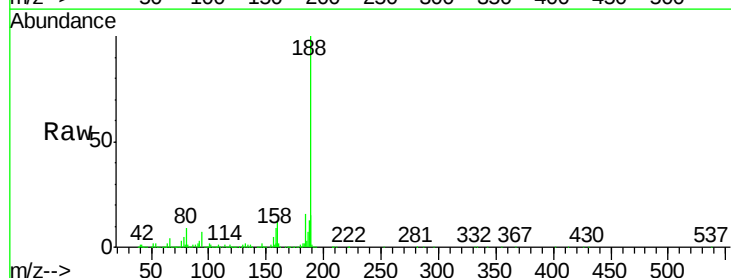


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

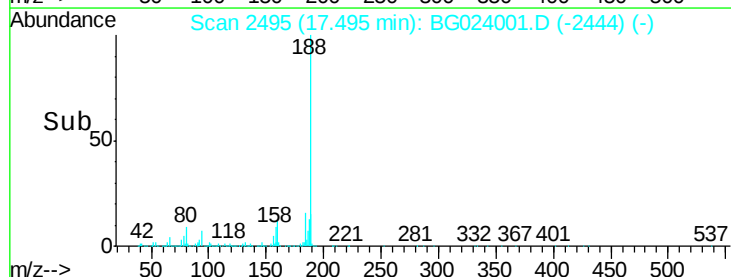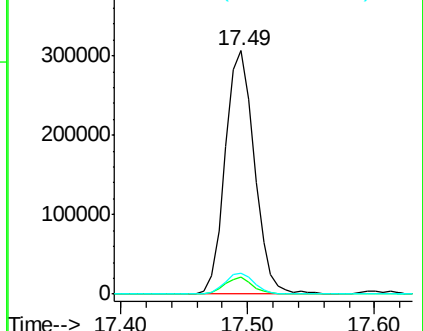

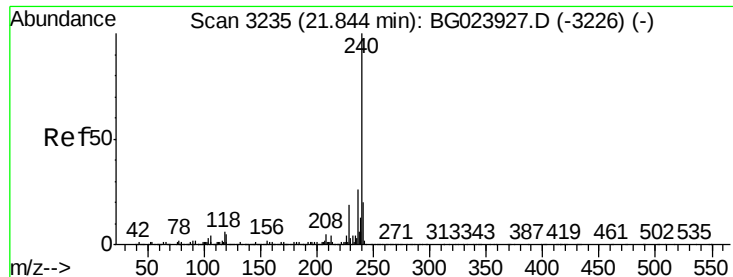

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.80 min Scan# 3228

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59

Instrument :

BNA_G

ClientSampleId :

BRC001-AT01-AQ002-01


Tot Ion:240 Resp: 491362

Ion Ratio Lower Upper

240 100

120 6.1 4.1 6.1




236 26.7 21.1 31.7

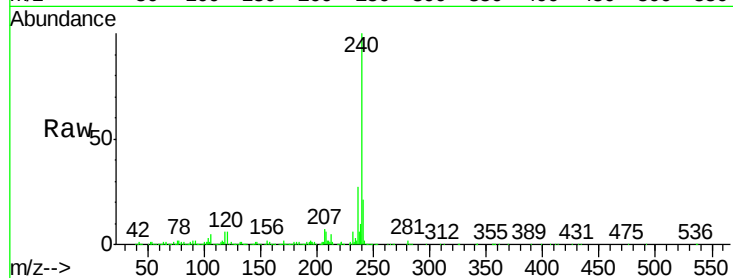

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

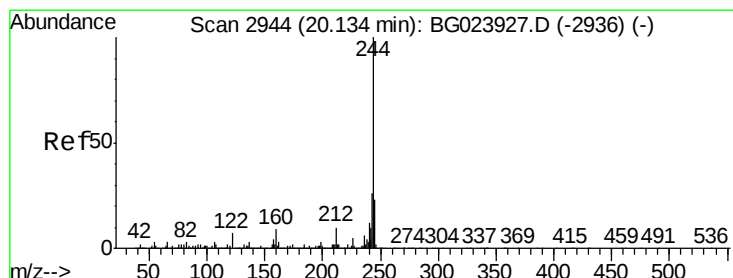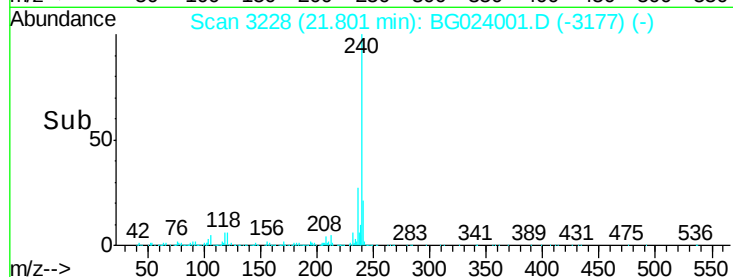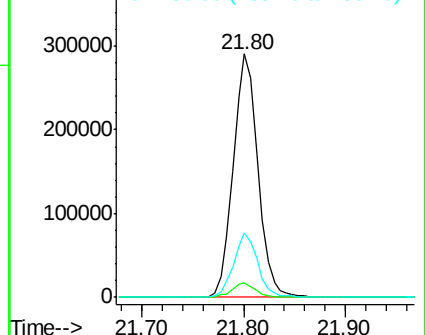

#78

Terphenyl-d14

Concen: 64.76 ng

RT: 20.10 min Scan# 2939

Delta R.T. -0.00 min

Lab File: BG024001.D

Acq: 16 Sep 2016 19:59


Tgt Ion:244 Resp: 1397202

Ion Ratio Lower Upper

244 100

212 10.7 10.8 16.2#



122 7.4 8.0 12.0#

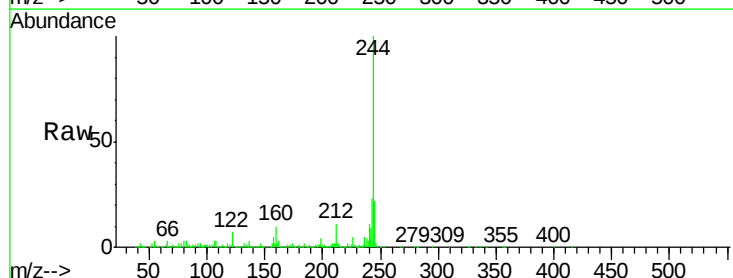


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

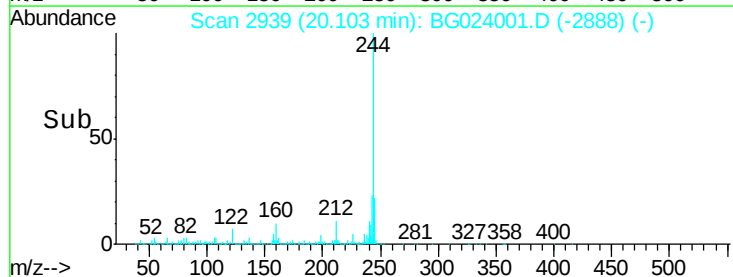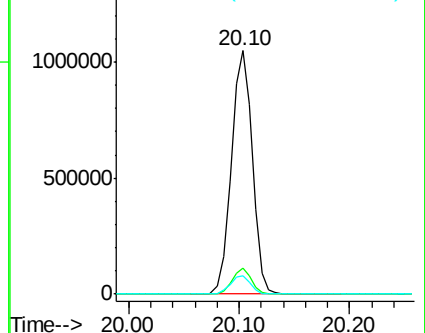

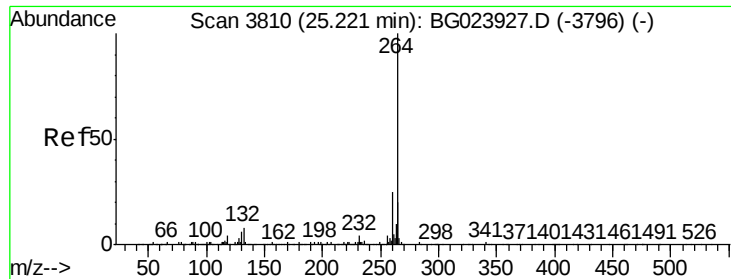

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.15 min Scan# 3798
Delta R.T. 0.00 min
Lab File: BG024001.D
Acq: 16 Sep 2016 19:59

Instrument :
BNA_G
ClientSampleId :
BRC001-AT01-AQ002-01

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.4	27.6
265	23.5	18.9	28.3

