


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091616\
Data File : BG023992.D
Acq On : 16 Sep 2016 14:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 09 16:24:09 2016

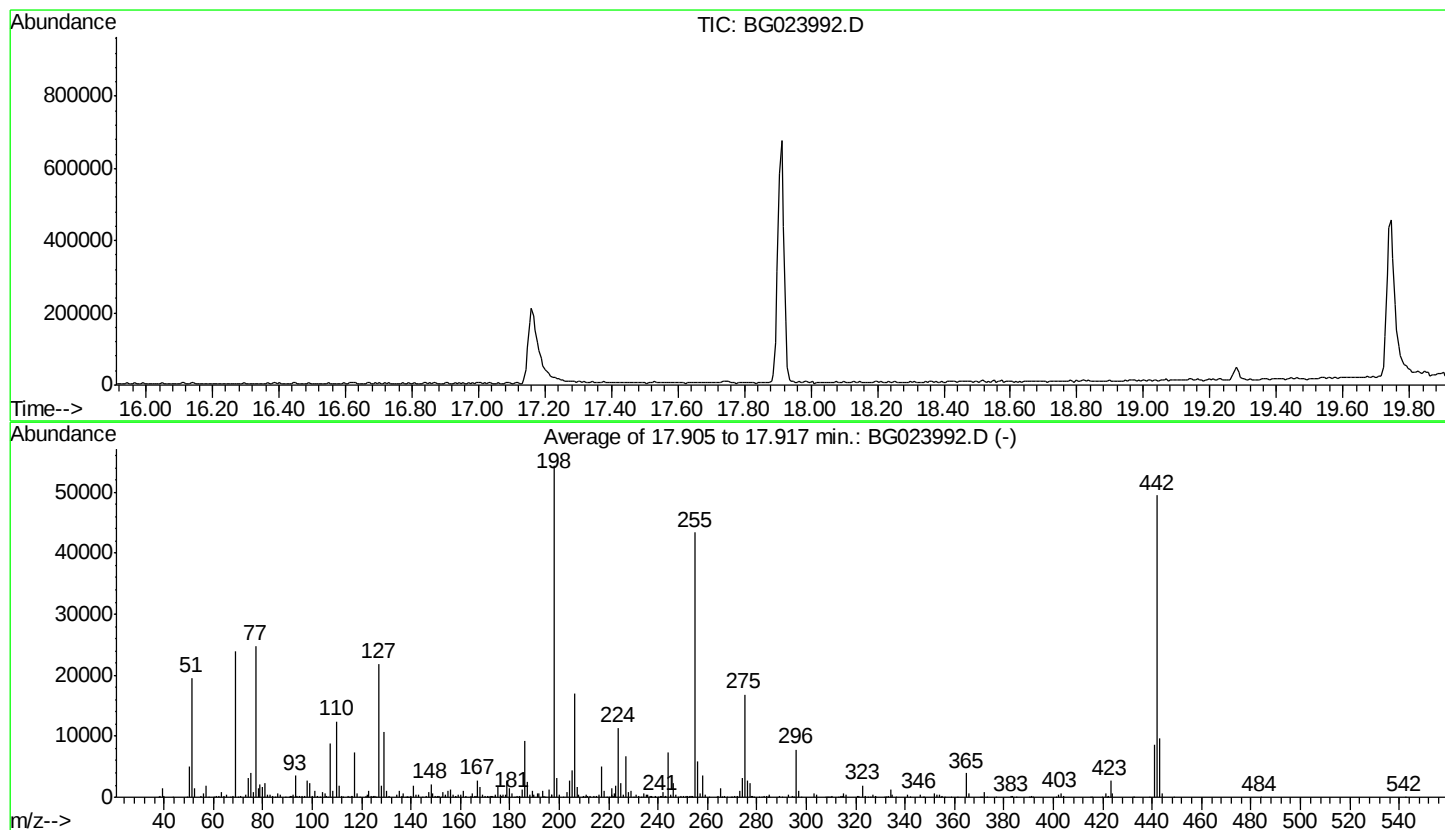

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	19559	PASS
68	69	0.00	2	1.3	306	PASS
69	198	0.00	100	43.9	23838	PASS
70	69	0.00	2	0.2	56	PASS
127	198	10	80	40.3	21932	PASS
197	198	0.00	2	0.8	454	PASS
198	198	100	100	100.0	54360	PASS
199	198	5	9	5.8	3132	PASS
275	198	10	60	31.1	16880	PASS
365	198	1	100	7.2	3934	PASS
441	442	0.01	24	17.5	8660	PASS
442	198	50	100	91.0	49458	PASS
443	442	15	24	19.7	9764	PASS