
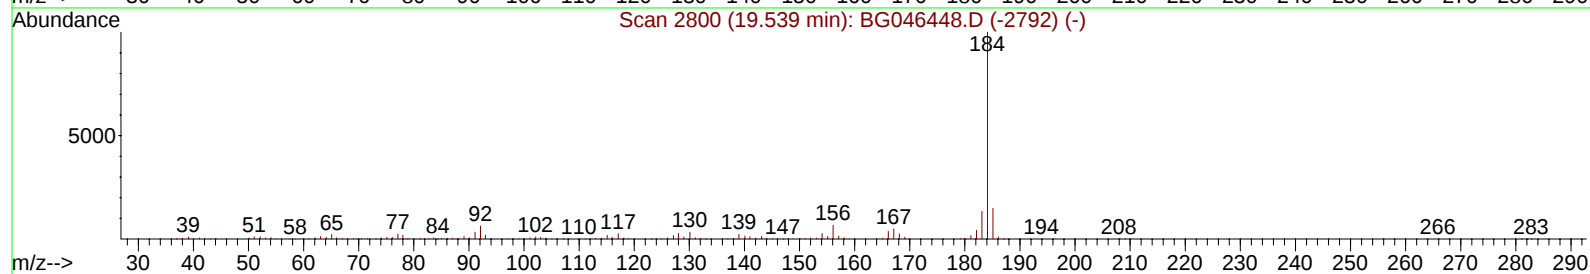
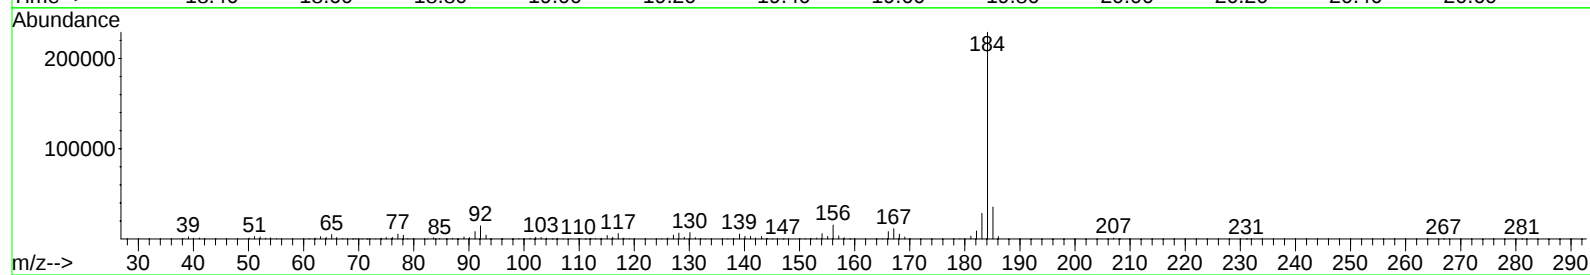


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091620\  
 Data File : BG046635.D  
 Acq On : 16 Sep 2020 8:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 17:57:52 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 16 11:07:52 2020  
 Response via : Initial Calibration

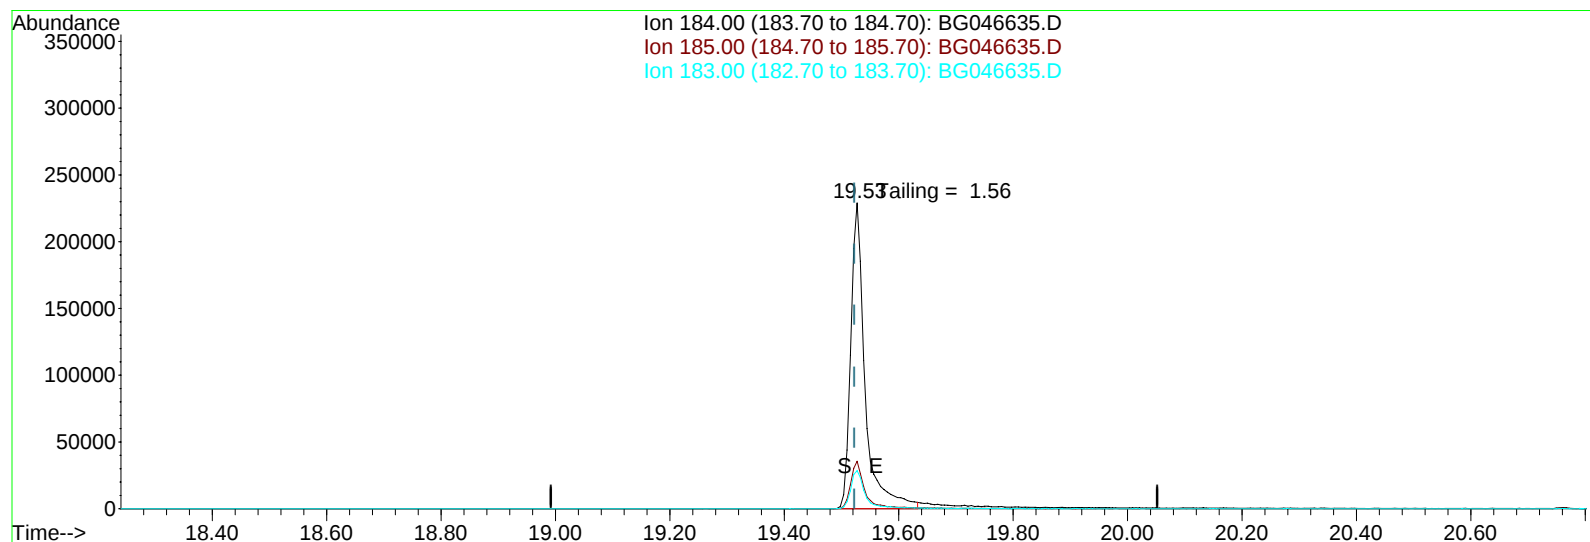

TIC: BG046635.D

(77) Benzidine




19.527min (+0.005) 96679.98ng

response 415611

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.50 | 15.54 |
| 183.00 | 13.20 | 12.44 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091620\  
Data File : BG046635.D  
Acq On : 16 Sep 2020 8:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 17:57:52 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 16 11:07:52 2020  
Response via : Initial Calibration

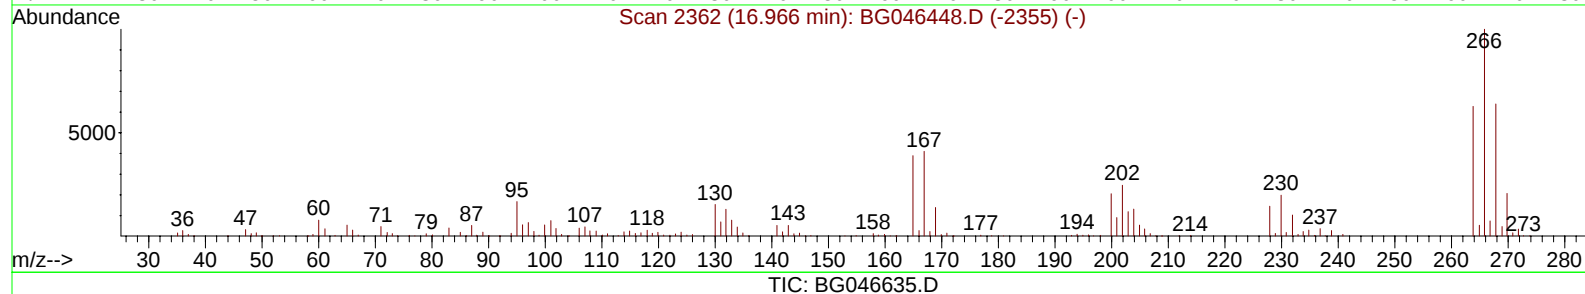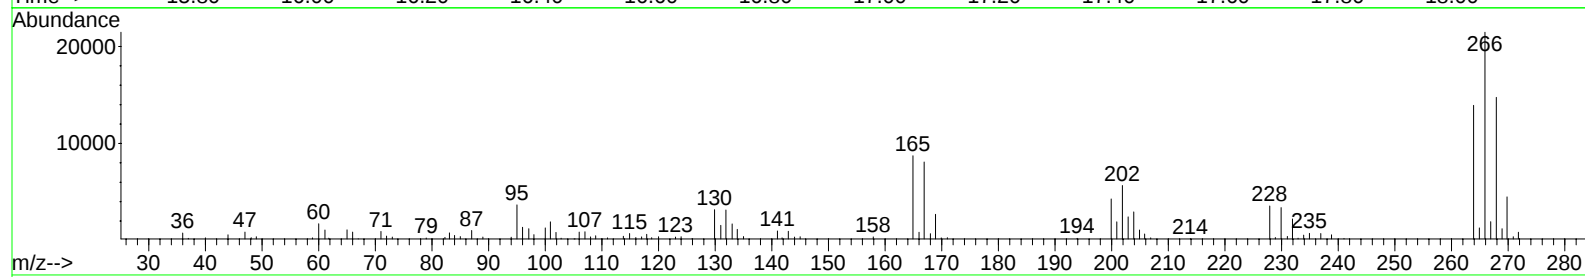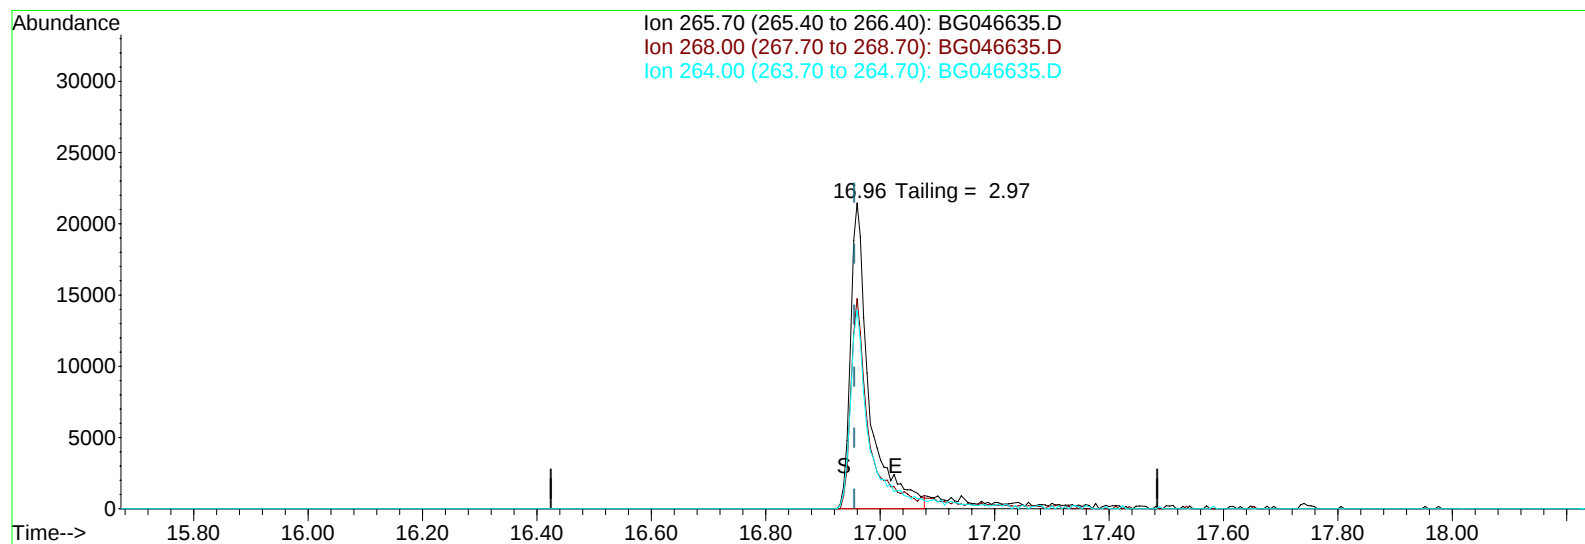

(70) Pentachlorophenol (C)

16.959min (+0.005) 61977.55ng

response 51463

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.20 | 68.73 |
| 264.00 | 61.60 | 64.89 |
| 0.00   | 0.00  | 0.00  |