
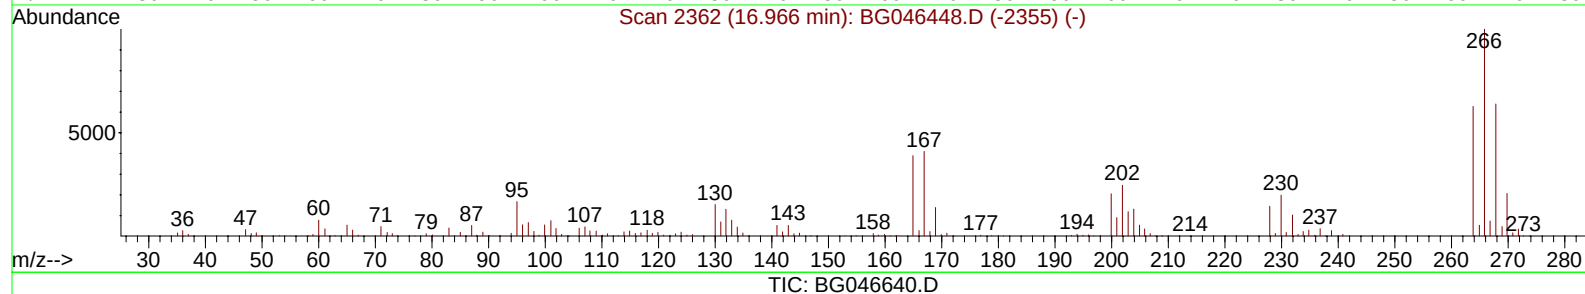
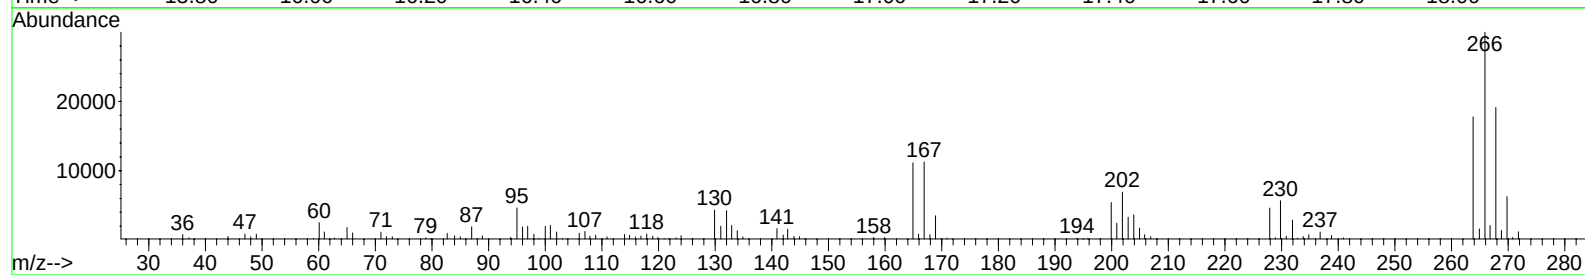


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091620\
Data File : BG046640.D
Acq On : 16 Sep 2020 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 17:54:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 16 11:07:52 2020
Response via : Initial Calibration

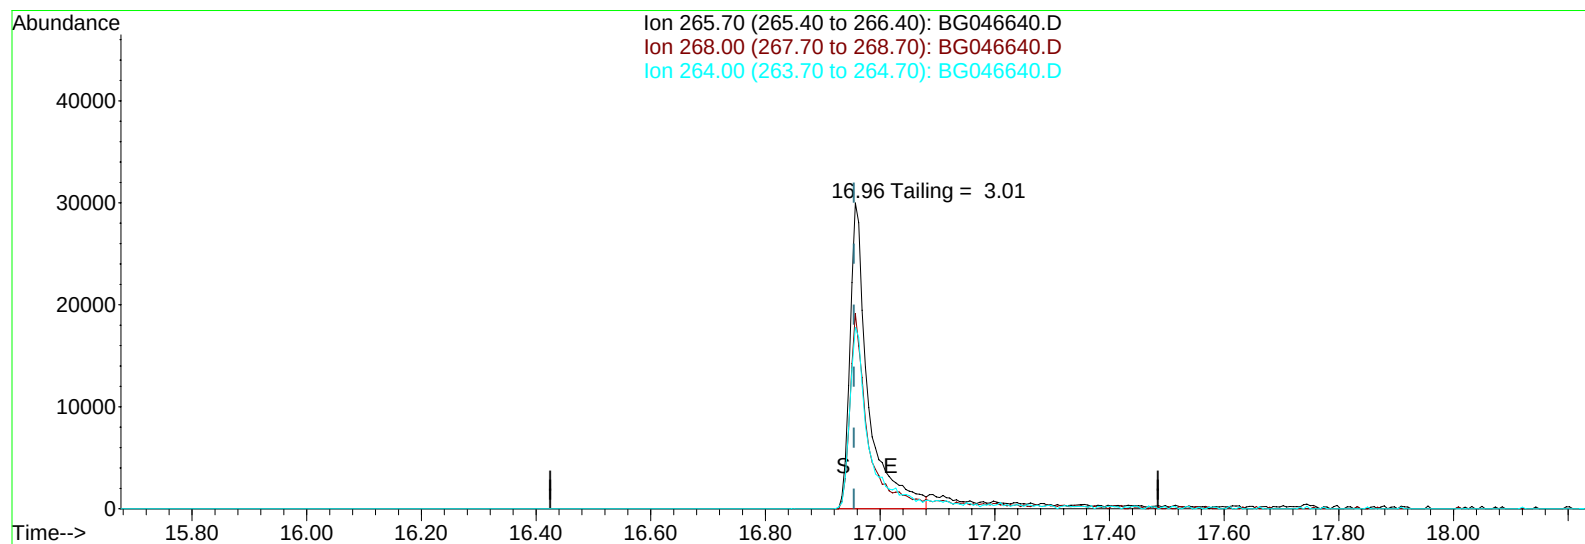

(70) Pentachlorophenol (C)




16.957min (+0.002) 24273.93ng

response 67350

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.82
264.00	61.60	59.28
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091620\
 Data File : BG046640.D
 Acq On : 16 Sep 2020 14:00
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 17:54:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 16 11:07:52 2020
 Response via : Initial Calibration

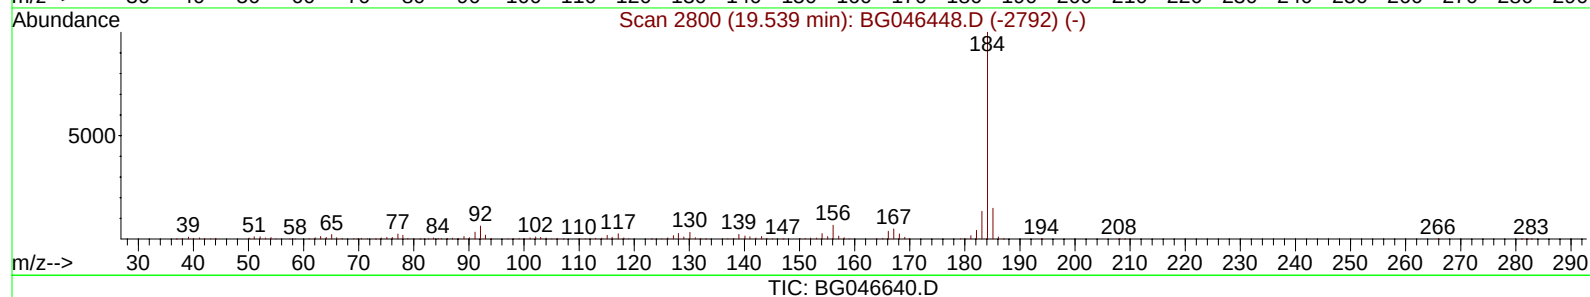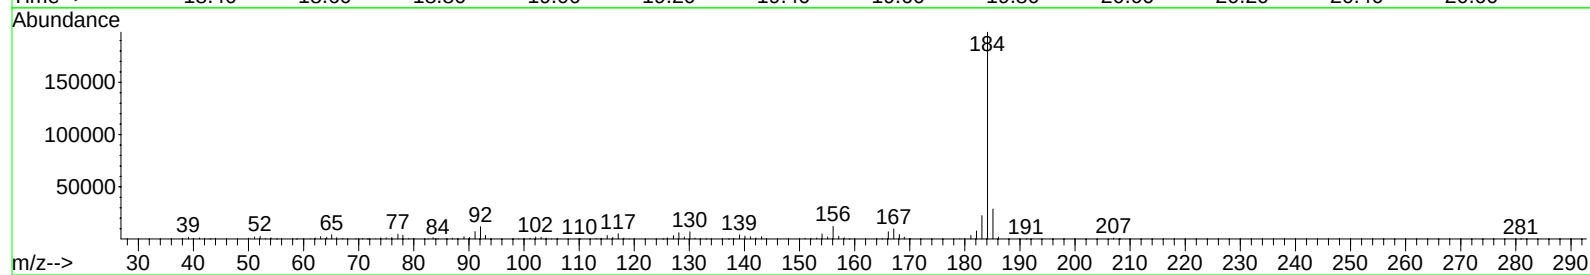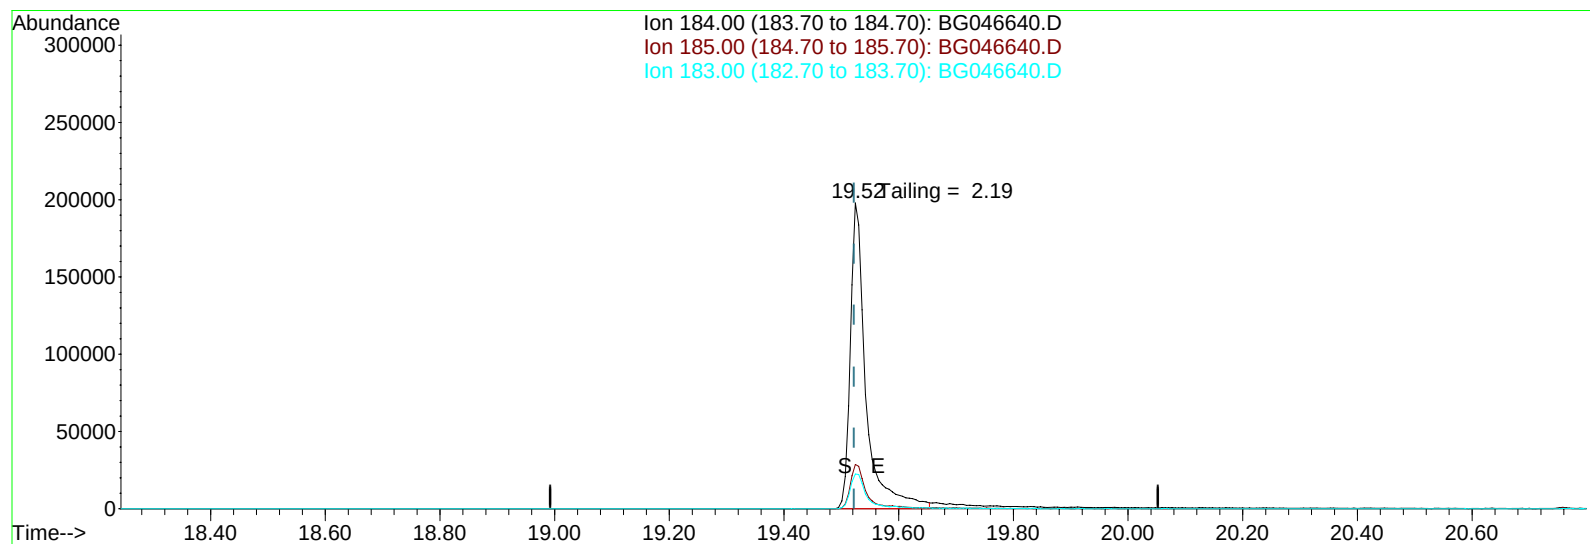

(77) Benzidine

19.524min (+0.002) 0.00ng

response 392344

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.51
183.00	13.20	11.38
0.00	0.00	0.00