


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091620\
 Data File : BG046640.D
 Acq On : 16 Sep 2020 14:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 16 11:07:52 2020

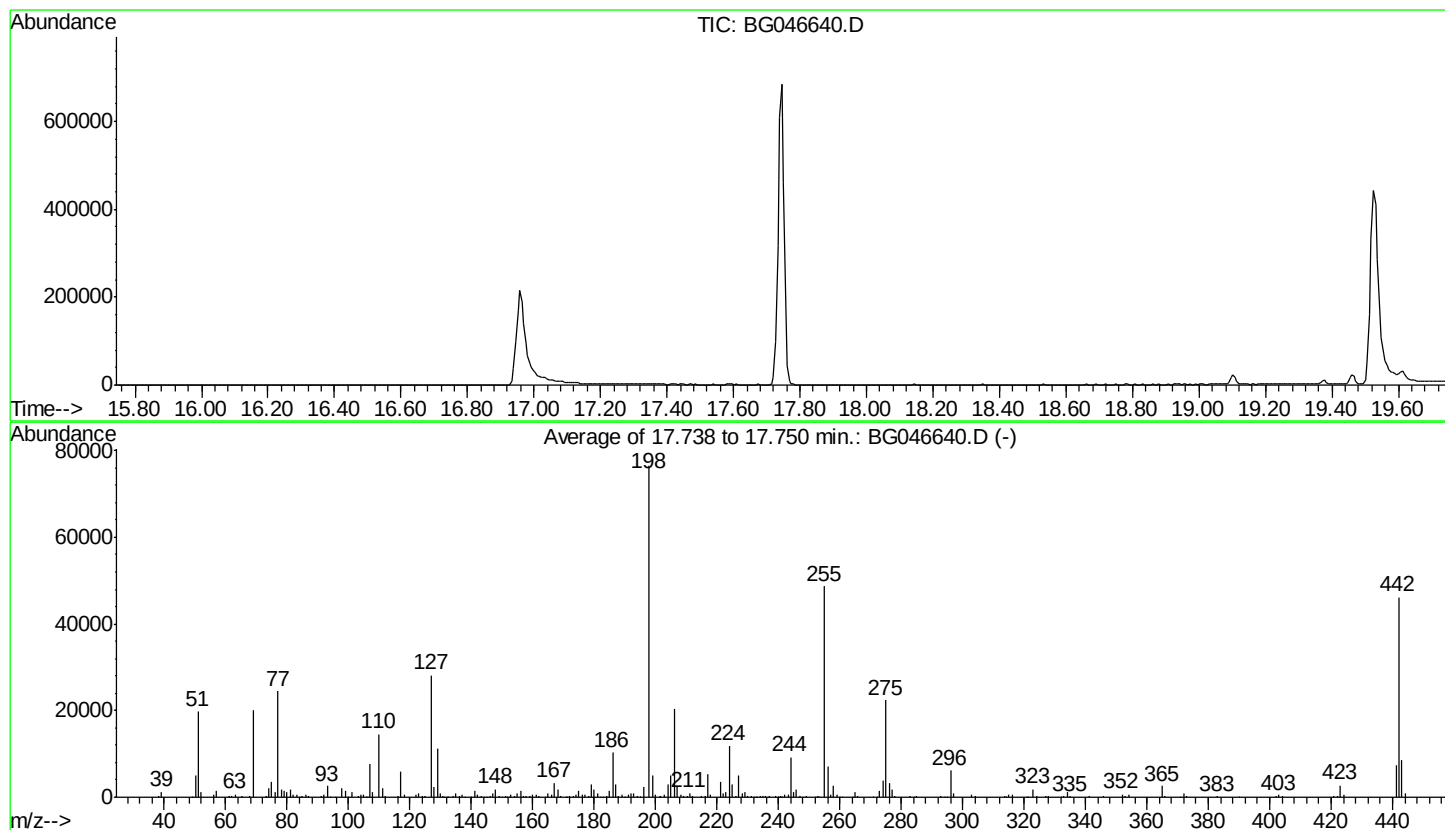

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	19682	PASS
68	69	0.00	2	1.0	194	PASS
69	198	0.00	100	26.2	20089	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.8	28202	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76538	PASS
199	198	5	9	6.8	5176	PASS
275	198	10	60	29.2	22370	PASS
365	198	1	100	3.3	2557	PASS
441	198	0.01	100	9.5	7259	PASS
442	198	50	100	60.4	46205	PASS
443	442	15	24	18.3	8439	PASS