

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064392.D
 Acq On : 16 Sep 2025 19:28
 Operator : RC/JU
 Sample : PB169690BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK690

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	44	rVB3	7467	11377	1.23%	0.139%
2	3.717	102	107	117	rBV	89820	149878	16.17%	1.833%
3	4.152	179	181	184	rVB3	1144	1331	0.14%	0.016%
4	6.261	535	540	544	rVB	820	1329	0.14%	0.016%
5	7.013	659	668	680	rBV	130564	220494	23.78%	2.696%
6	7.172	689	695	703	rVB	66585	111444	12.02%	1.363%
7	7.377	724	730	741	rVB	125122	210183	22.67%	2.570%
8	7.841	803	809	816	rBV2	69369	115767	12.49%	1.415%
9	8.546	922	929	937	rBV2	157323	264654	28.55%	3.236%
10	8.993	996	1005	1019	rBV	109453	194304	20.96%	2.376%
11	9.710	1121	1127	1135	rBV	106661	186141	20.08%	2.276%
12	10.250	1212	1219	1234	rBV	146807	266334	28.73%	3.256%
13	10.626	1276	1283	1292	rVB	90754	160061	17.27%	1.957%
14	10.761	1298	1306	1319	rBV	134162	245791	26.51%	3.005%
15	12.219	1550	1554	1561	rBV2	1550	3183	0.34%	0.039%
16	13.875	1830	1836	1842	rBV	306487	423926	45.73%	5.183%
17	14.157	1876	1884	1892	rBV2	286710	449041	48.44%	5.490%
18	14.469	1929	1937	1943	rBV	146355	226038	24.38%	2.764%
19	14.663	1964	1970	1988	rBV	125378	225387	24.31%	2.756%
20	15.462	2099	2106	2114	rBV	370475	572601	61.76%	7.001%
21	15.573	2120	2125	2138	rBV	114229	184891	19.94%	2.261%
22	15.697	2144	2146	2152	rVB3	2470	3344	0.36%	0.041%
23	16.995	2363	2367	2368	rBV	1352	1353	0.15%	0.017%
24	17.207	2396	2403	2412	rBV	219144	321118	34.64%	3.926%
25	17.307	2412	2420	2429	rBV2	481050	696659	75.15%	8.518%
26	19.157	2730	2735	2740	rVB5	6558	10292	1.11%	0.126%
27	19.228	2742	2747	2752	rVB2	6389	9778	1.05%	0.120%
28	19.481	2788	2790	2795	rVB3	1072	1205	0.13%	0.015%
29	19.534	2795	2799	2801	rBV	1292	1250	0.13%	0.015%
30	19.592	2803	2809	2819	rVV	624280	879596	94.88%	10.755%
31	19.680	2821	2824	2825	rBV2	1716	1563	0.17%	0.019%
32	20.009	2877	2880	2882	rBV2	1379	1463	0.16%	0.018%
33	20.203	2910	2913	2916	rBV3	1857	2388	0.26%	0.029%
34	20.321	2929	2933	2934	rBV3	1505	1600	0.17%	0.020%
35	20.450	2953	2955	2956	rBV	1755	1309	0.14%	0.016%
36	20.568	2974	2975	2977	rBV2	2376	1603	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
 Data File : BG064392.D
 Acq On : 16 Sep 2025 19:28
 Operator : RC/JU
 Sample : PB169690BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK690

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
 Title : SVOA CALIBRATION

37	20.615	2981	2983	2985	rBV3	1548	1907	0.21%	0.023%
38	20.791	3011	3013	3016	rBV2	1692	1815	0.20%	0.022%
39	21.431	3116	3122	3131	rBV2	265074	427260	46.09%	5.224%
40	22.201	3251	3253	3258	rVB5	6970	6685	0.72%	0.082%
41	22.765	3347	3349	3352	rBV3	2700	3505	0.38%	0.043%
42	22.847	3359	3363	3368	rVB4	12676	19583	2.11%	0.239%
43	22.930	3375	3377	3380	rVB3	3147	2285	0.25%	0.028%
44	22.965	3380	3383	3384	rBV3	3071	3415	0.37%	0.042%
45	23.306	3439	3441	3442	rBV2	2529	1497	0.16%	0.018%
46	23.593	3484	3490	3496	rBV5	15314	31009	3.34%	0.379%
47	23.922	3544	3546	3549	rBV3	2947	2605	0.28%	0.032%
48	24.228	3588	3598	3607	rBV	366423	927081	100.00%	11.335%
49	24.434	3624	3633	3645	rVB	167439	480819	51.86%	5.879%
50	25.497	3808	3814	3816	rBV4	17127	32146	3.47%	0.393%
51	25.750	3855	3857	3858	rBV2	2827	1714	0.18%	0.021%
52	26.737	4019	4025	4033	rVB9	14811	40376	4.36%	0.494%
53	26.937	4058	4059	4061	rBV2	3190	1382	0.15%	0.017%
54	28.229	4275	4279	4286	rVB9	10430	23492	2.53%	0.287%
55	28.617	4343	4345	4347	rBV3	3509	2926	0.32%	0.036%
56	28.717	4360	4362	4363	rBV2	2878	1322	0.14%	0.016%
57	28.734	4363	4365	4367	rBV3	3425	2612	0.28%	0.032%
58	29.998	4579	4580	4582	rBV2	5051	4718	0.51%	0.058%


Sum of corrected areas: 8178830

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064392.D
Acq On : 16 Sep 2025 19:28
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

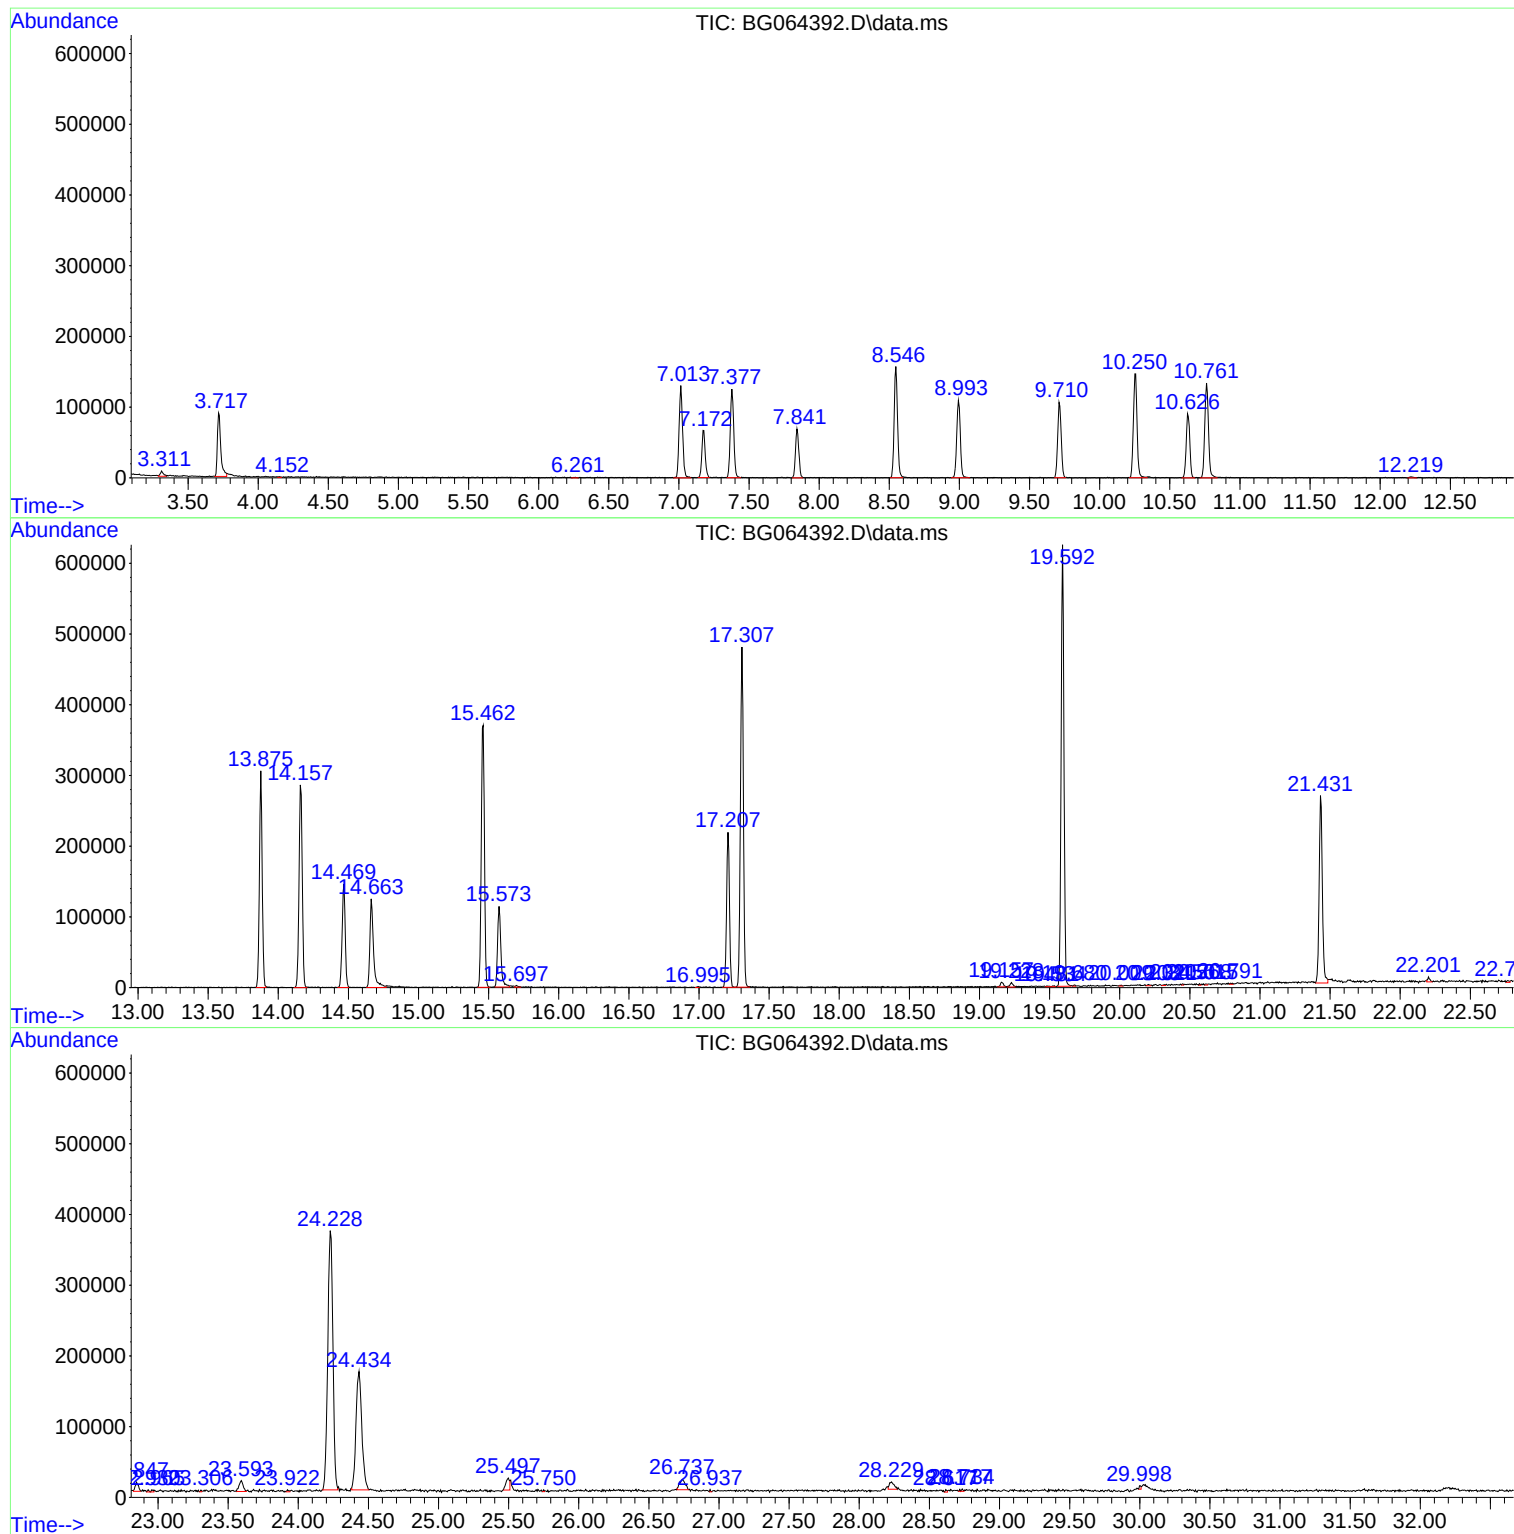

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064392.D
Acq On : 16 Sep 2025 19:28
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091625\
Data File : BG064392.D
Acq On : 16 Sep 2025 19:28
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091125.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc