
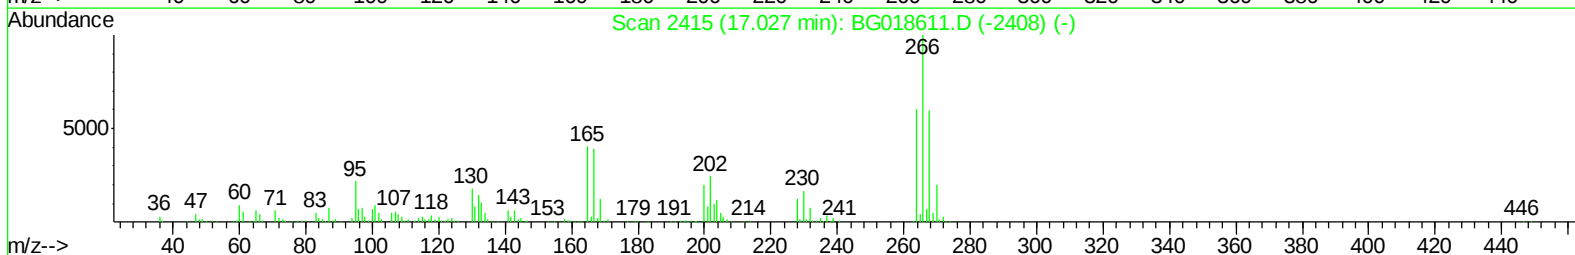
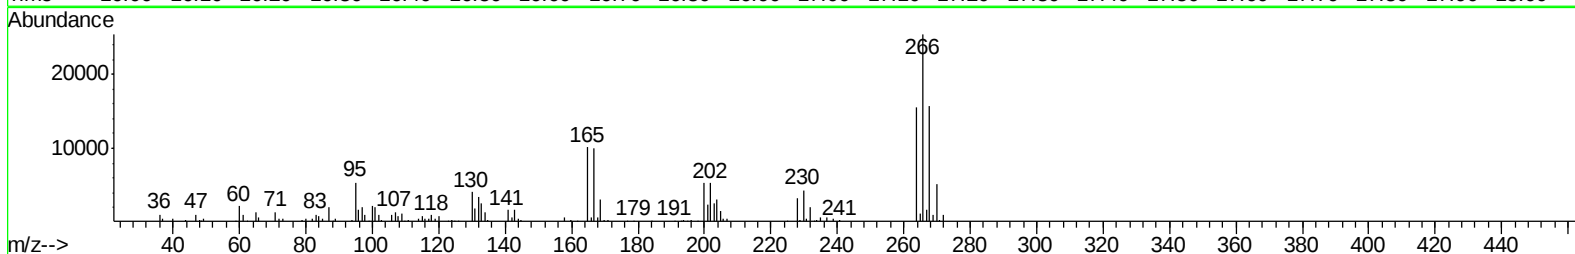


Data Path : Z:\HPCHEM1\BNA_G\Data\BG091715\
Data File : BG018709.D
Acq On : 16 Sep 2015 17:07
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 17:03:20 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 10:44:16 2015
Response via : Initial Calibration

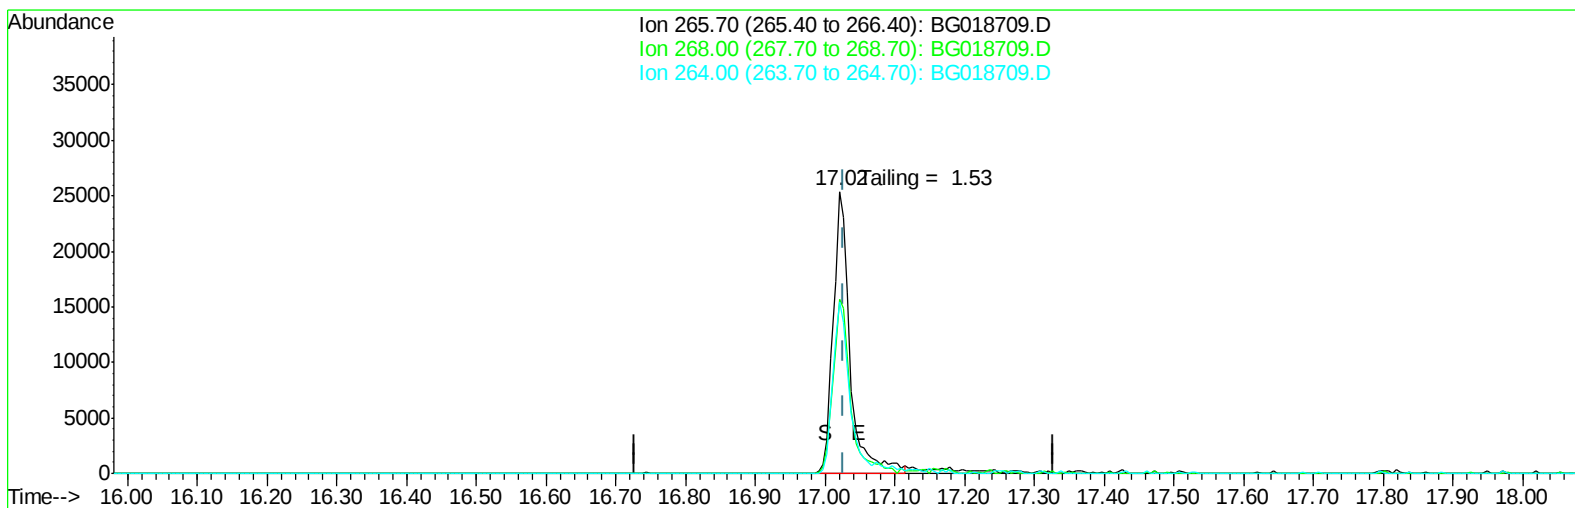

TIC: BG018709.D

(69) Pentachlorophenol (C)




17.020min (-0.007) 0.00ng

response 41413

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.79
264.00	60.10	60.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG091715\
Data File : BG018709.D
Acq On : 16 Sep 2015 17:07
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 17:03:20 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 11 10:44:16 2015
Response via : Initial Calibration

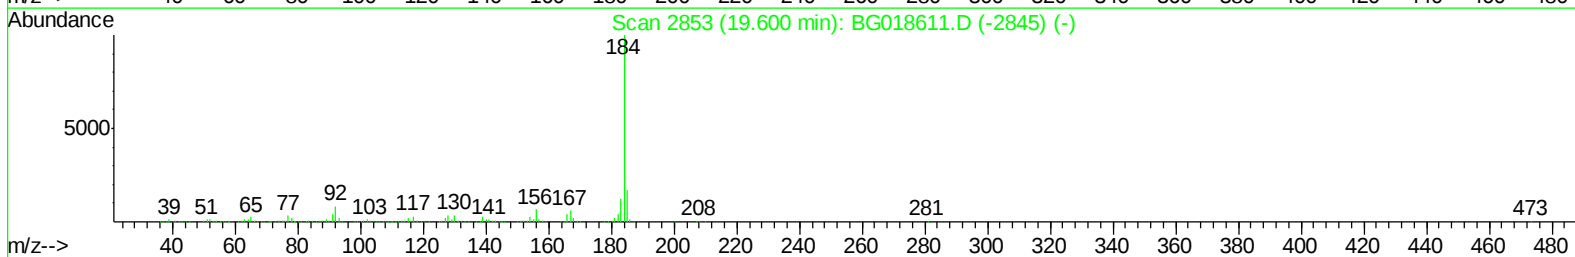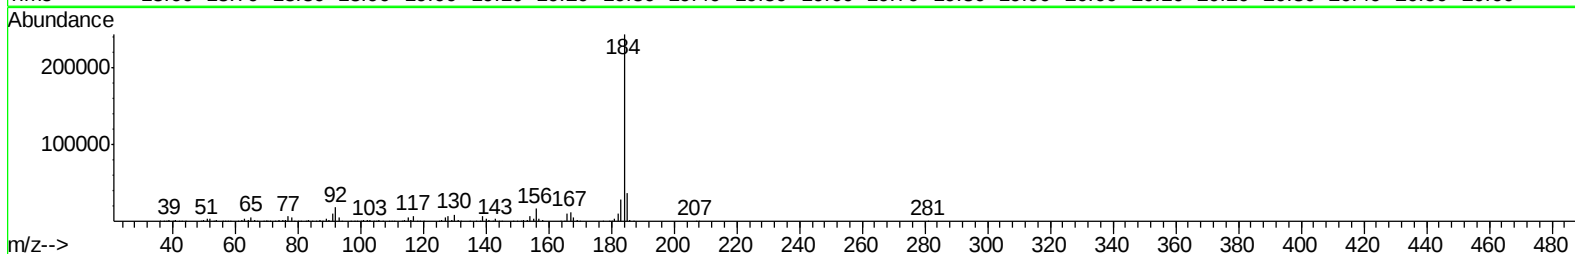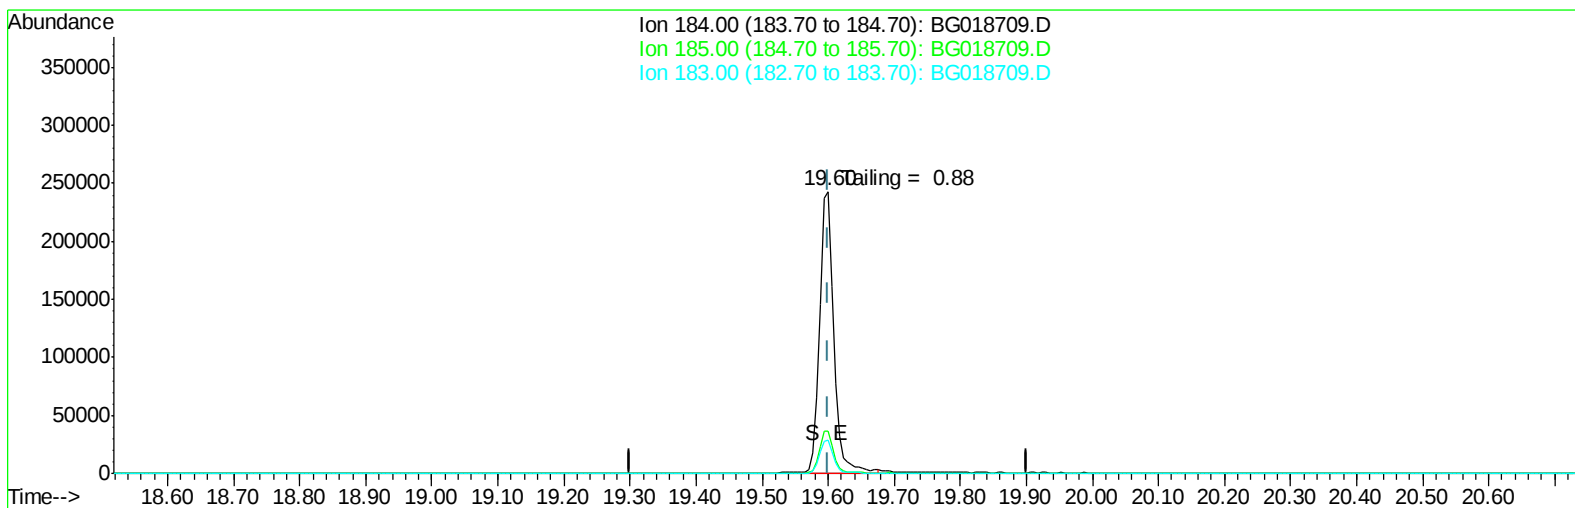

TIC: BG018709.D

(76) Benzidine

19.600min (-0.001) 0.00ng

response 371430

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.92
183.00	12.60	11.64
0.00	0.00	0.00