
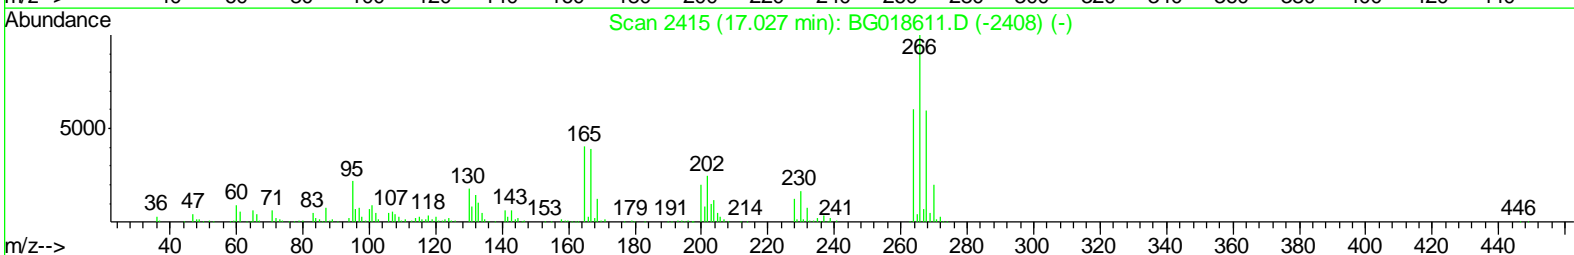
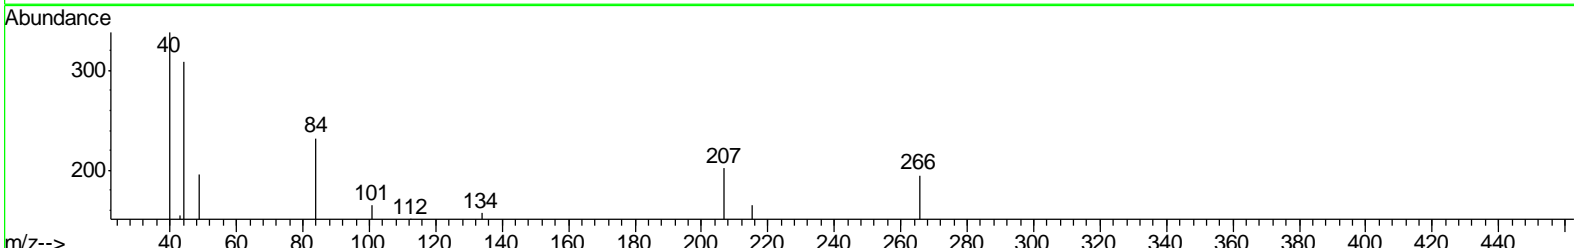


Data Path : Z:\HPCHEM1\BNA_G\Data\BG091715\
 Data File : BG018724.D
 Acq On : 17 Sep 2015 2:37
 Operator : TP
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 17:08:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 11 10:44:16 2015
 Response via : Initial Calibration

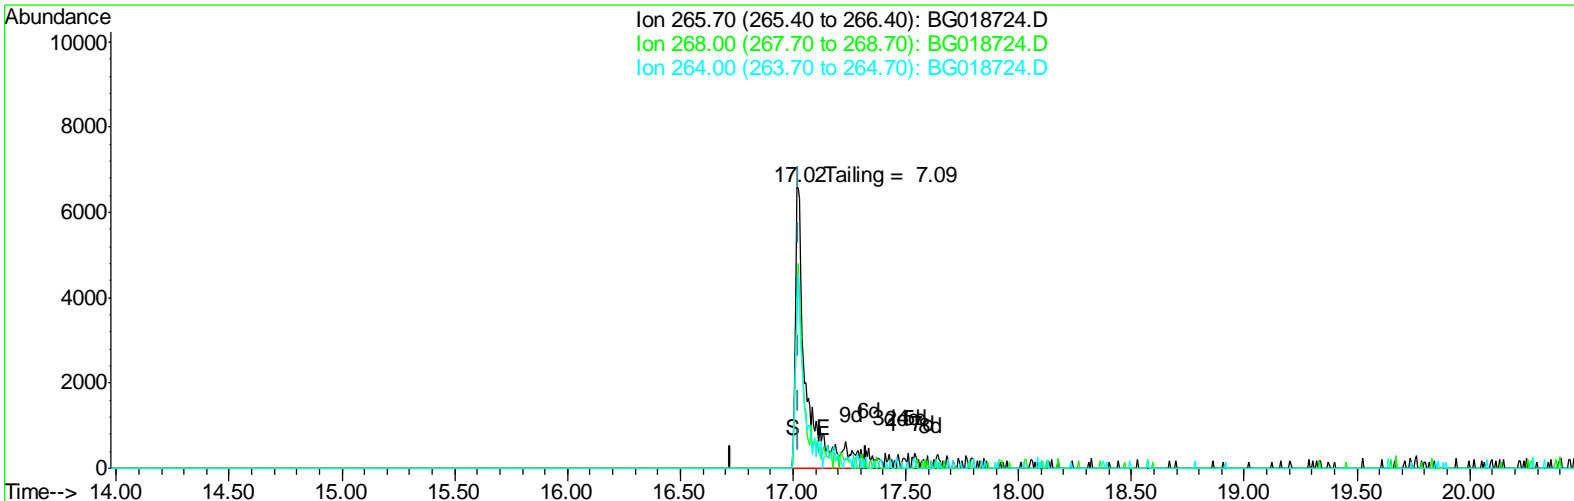




TIC: BG018724.D

(69) Pentachlorophenol (C)
 17.448min (+0.420) 112.36ng
 response 134

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	0.00#
264.00	60.10	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG091715\
 Data File : BG018724.D
 Acq On : 17 Sep 2015 2:37
 Operator : TP
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 17:08:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 11 10:44:16 2015
 Response via : Initial Calibration

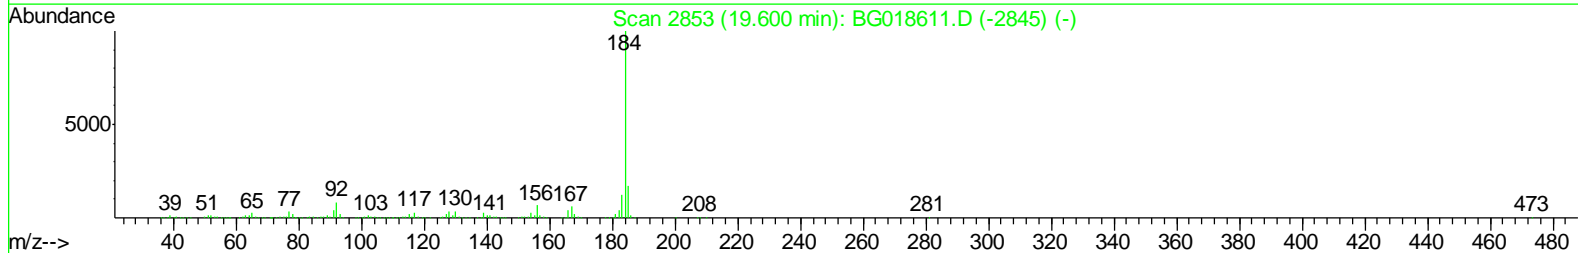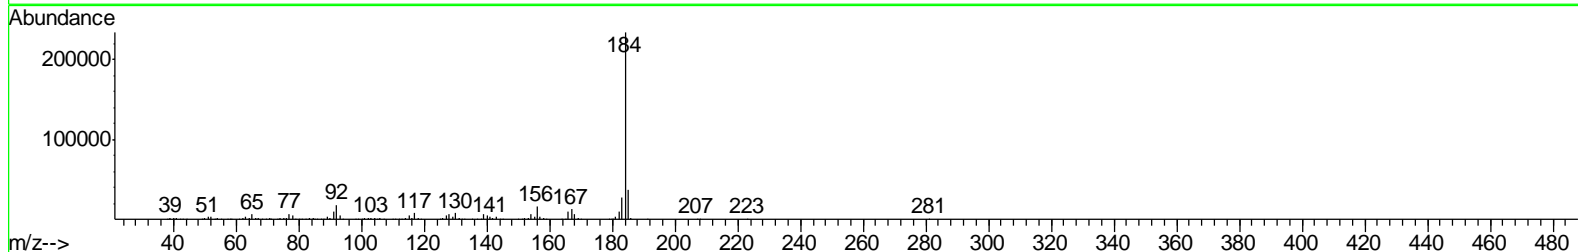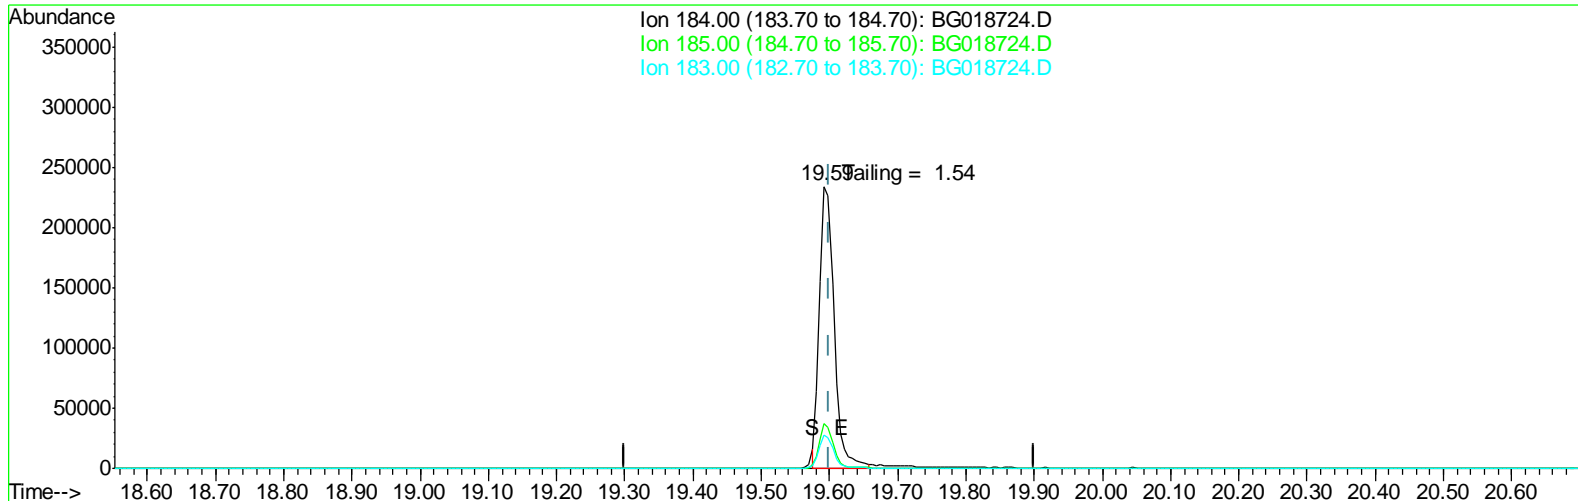

TIC: BG018724.D

(76) Benzidine

19.592min (-0.009) 0.00ng

response 359825

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.73
183.00	12.60	11.96
0.00	0.00	0.00