


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091715\
 Data File : BG018709.D
 Acq On : 16 Sep 2015 17:07
 Operator : TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

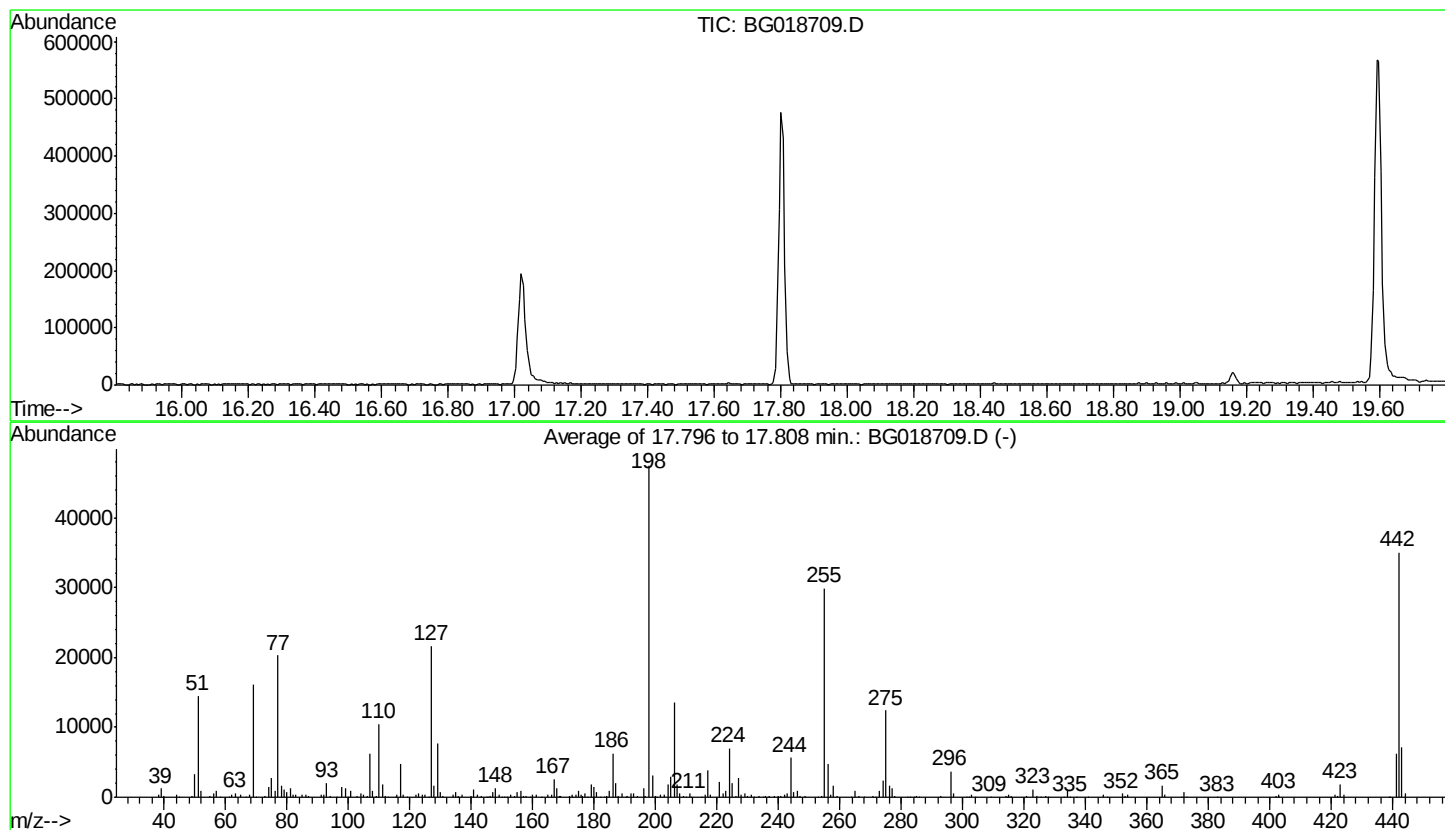

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	14523	PASS
68	69	0.00	2	2.0	319	PASS
69	198	0.00	100	34.1	16156	PASS
70	69	0.00	2	0.4	66	PASS
127	198	10	80	45.7	21658	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47440	PASS
199	198	5	9	6.4	3028	PASS
275	198	10	60	26.1	12376	PASS
365	198	1	100	3.5	1682	PASS
441	442	0.01	24	17.6	6157	PASS
442	198	50	100	73.9	35072	PASS
443	442	15	24	20.1	7060	PASS