


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091715\
 Data File : BG018724.D
 Acq On : 17 Sep 2015 2:37
 Operator : TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

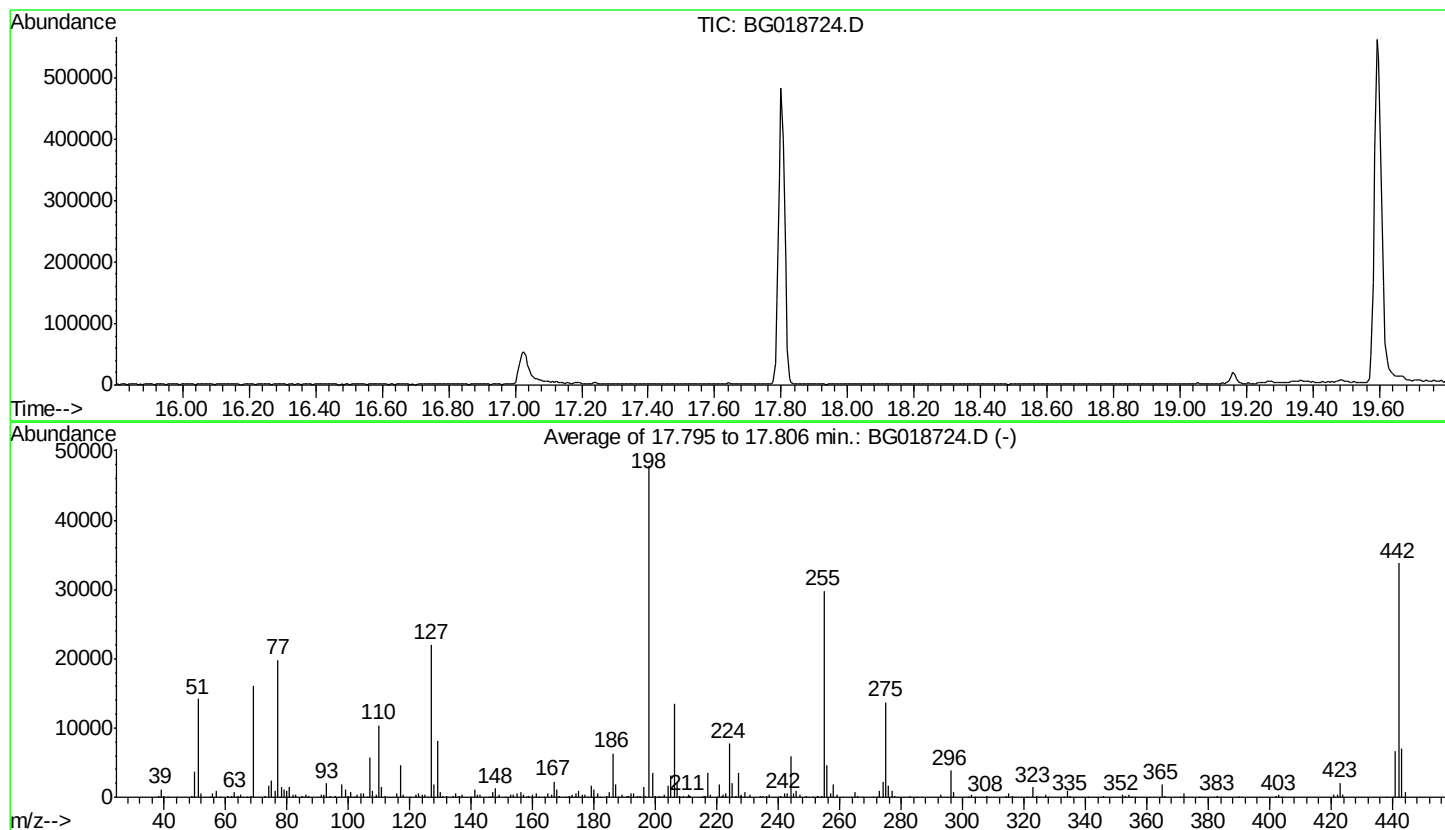

AutoFind: Scans 2545, 2546, 2547; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	14146	PASS
68	69	0.00	2	0.9	150	PASS
69	198	0.00	100	33.7	16115	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	22002	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47866	PASS
199	198	5	9	7.3	3481	PASS
275	198	10	60	28.6	13702	PASS
365	198	1	100	3.8	1817	PASS
441	442	0.01	24	19.7	6652	PASS
442	198	50	100	70.5	33744	PASS
443	442	15	24	20.8	7009	PASS