


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091719\
 Data File : BG042867.D
 Acq On : 17 Sep 2019 14:19
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:06:09 2019

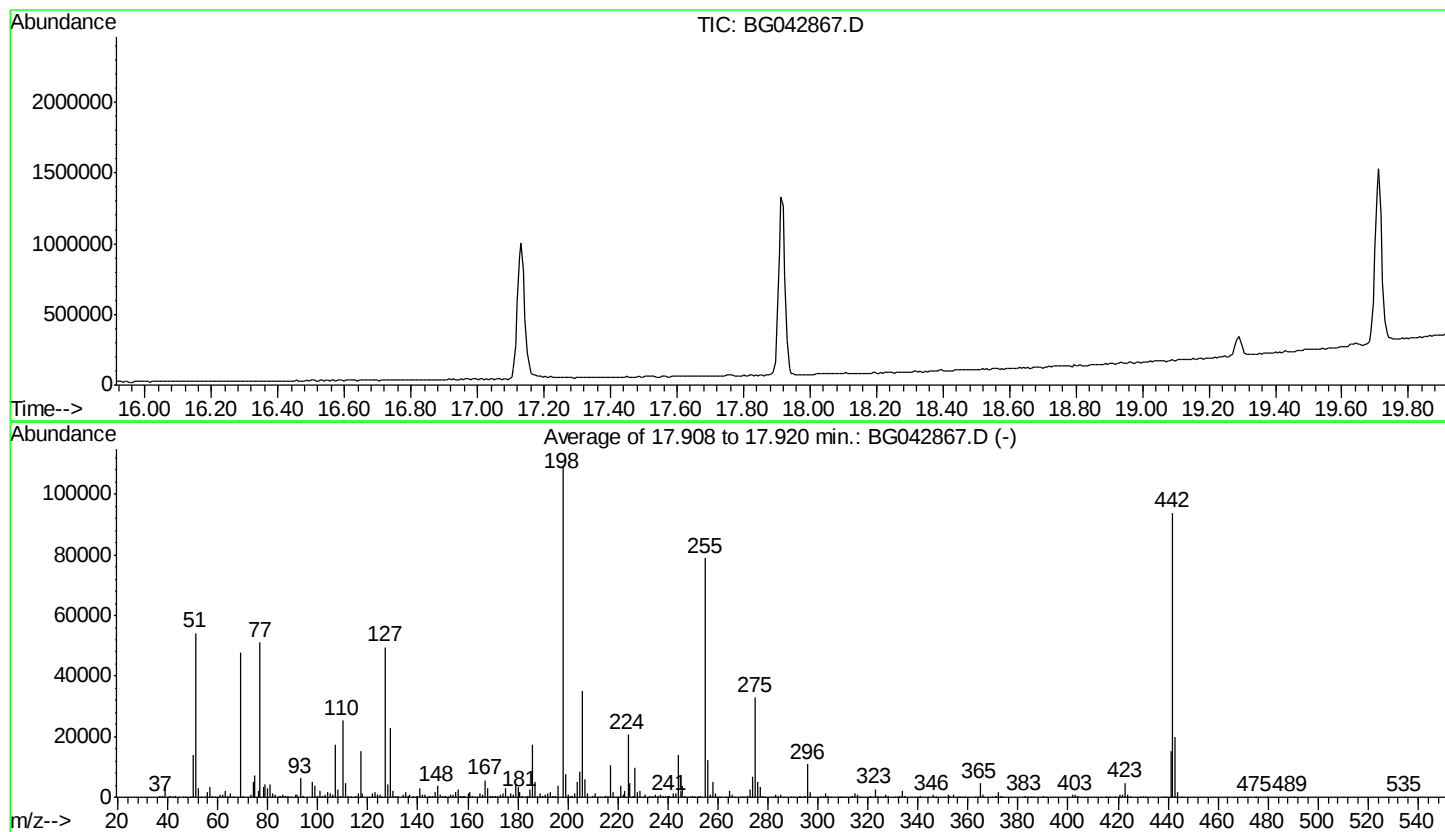

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	54234	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	47975	PASS
70	69	0.00	2	0.4	210	PASS
127	198	10	80	45.3	49594	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109474	PASS
199	198	5	9	7.1	7786	PASS
275	198	10	60	30.0	32797	PASS
365	198	1	100	4.2	4642	PASS
441	198	0.01	100	14.1	15429	PASS
442	198	50	100	85.9	94034	PASS
443	442	15	24	21.3	20036	PASS