
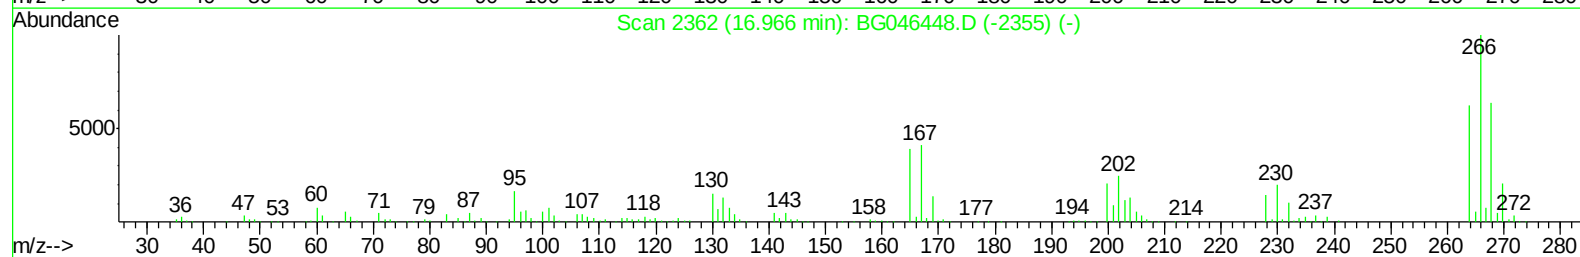
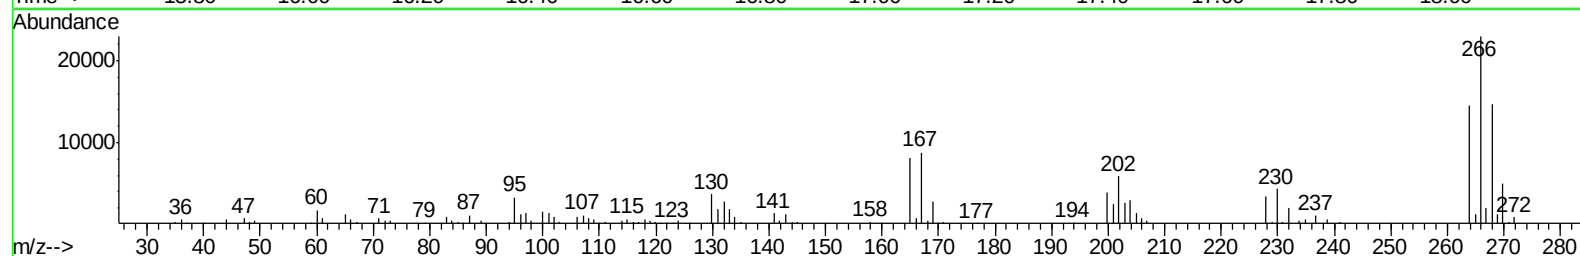


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091720\
Data File : BG046657.D
Acq On : 17 Sep 2020 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:34:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 17 14:27:03 2020
Response via : Initial Calibration

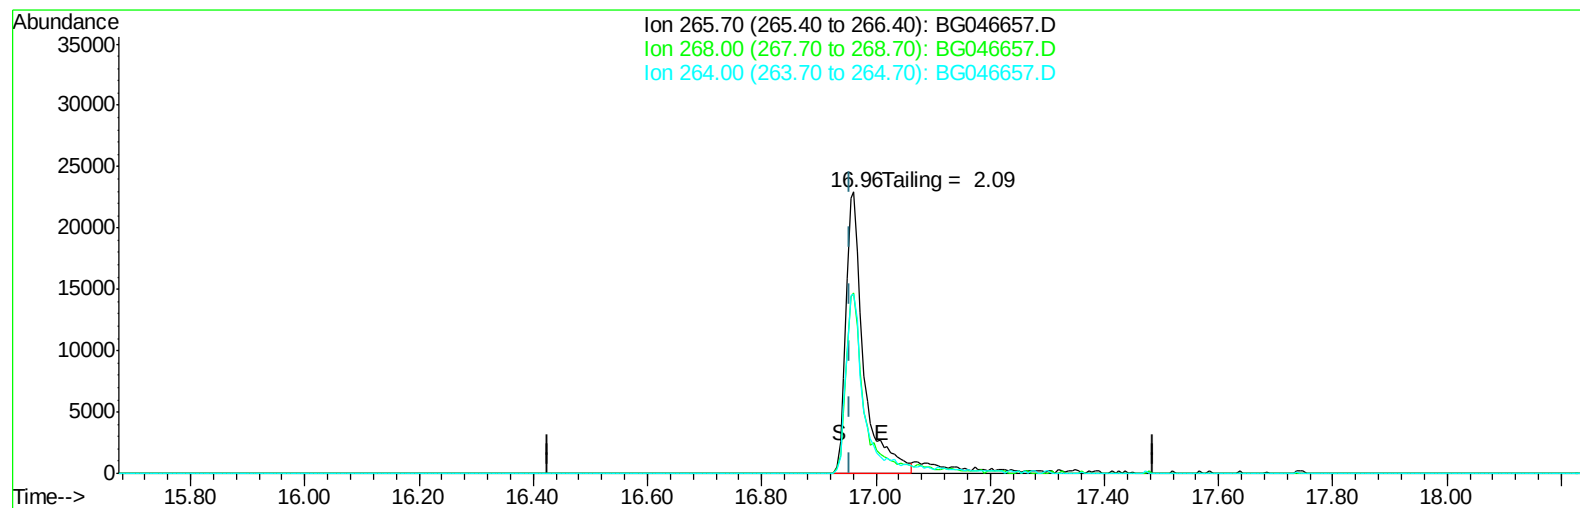

TIC: BG046657.D

(70) Pentachlorophenol (C)




16.961min (+0.005) 123866.69ng

response 50172

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.30
264.00	61.60	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091720\
 Data File : BG046657.D
 Acq On : 17 Sep 2020 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:34:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 17 14:27:03 2020
 Response via : Initial Calibration

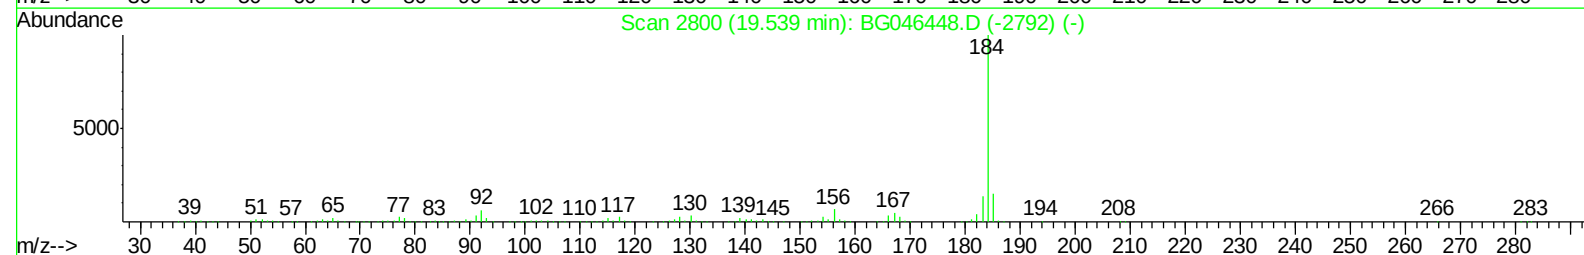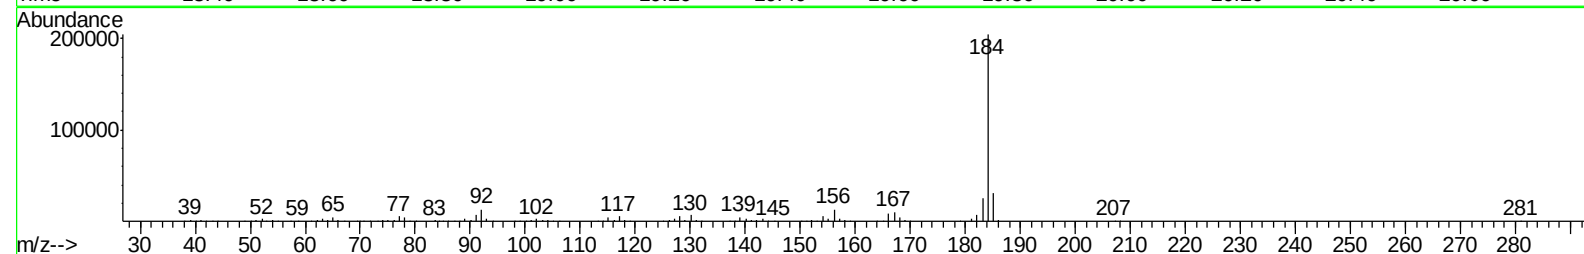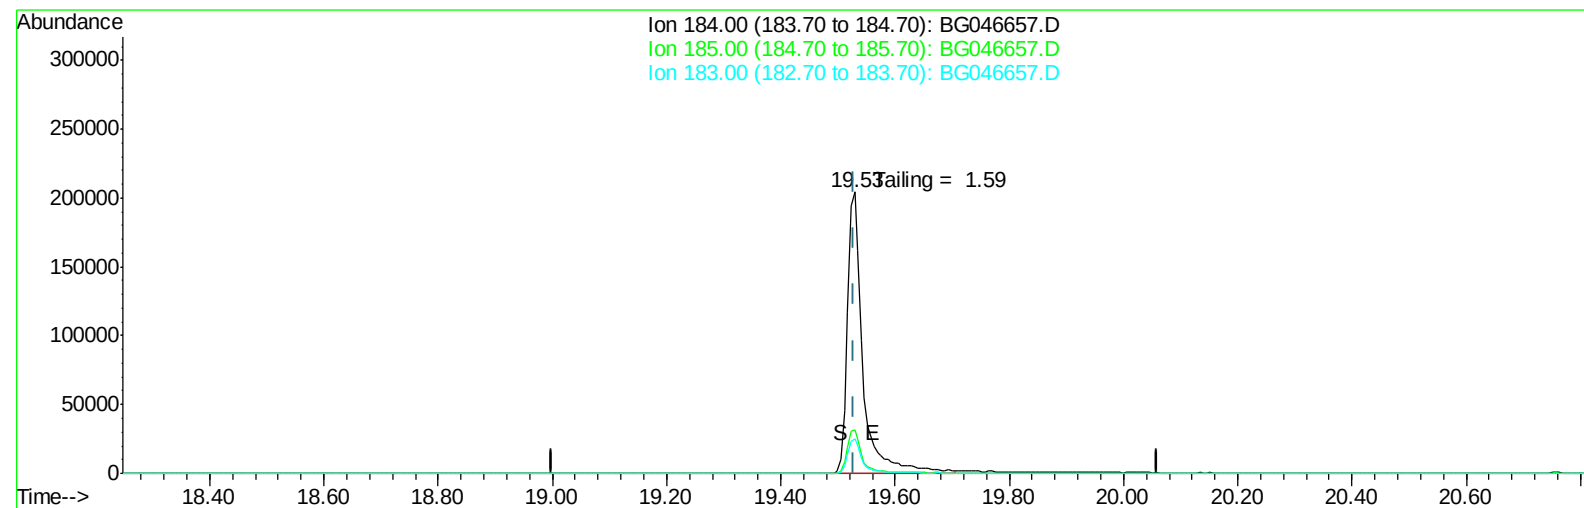

TIC: BG046657.D

(77) Benzidine

19.529min (-0.001) 0.00ng

response 387074

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.27
183.00	13.20	12.30
0.00	0.00	0.00