


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091720\
 Data File : BG046661.D
 Acq On : 17 Sep 2020 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 17 14:27:03 2020

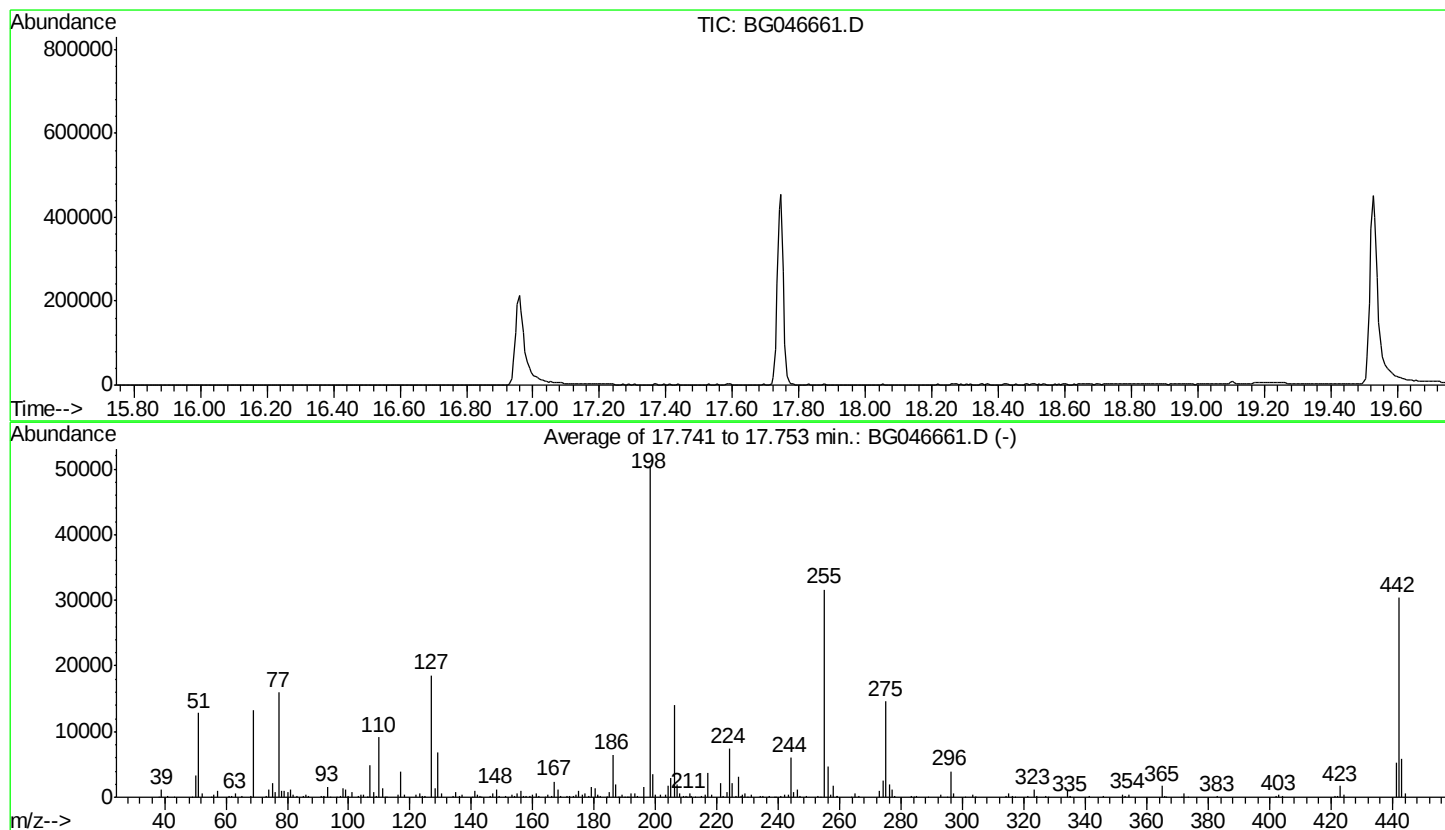

Spectrum Information: Average of 17.741 to 17.753 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	12783	PASS
68	69	0.00	2	0.8	109	PASS
69	198	0.00	100	26.1	13194	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.7	18563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50522	PASS
199	198	5	9	7.1	3572	PASS
275	198	10	60	28.8	14544	PASS
365	198	1	100	3.4	1715	PASS
441	198	0.01	100	10.3	5180	PASS
442	198	50	100	60.1	30368	PASS
443	442	15	24	19.5	5920	PASS