
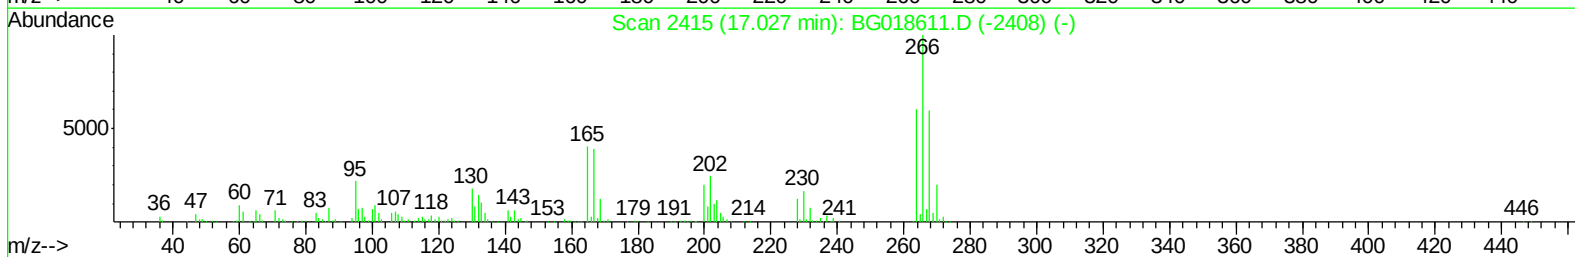
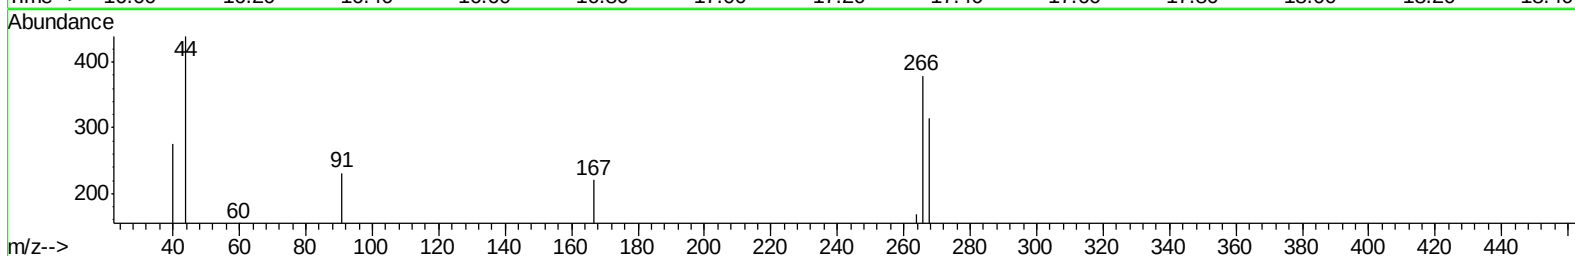


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091815\
Data File : BG018745.D
Acq On : 17 Sep 2015 19:35
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 04:19:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 03:41:39 2015
Response via : Initial Calibration

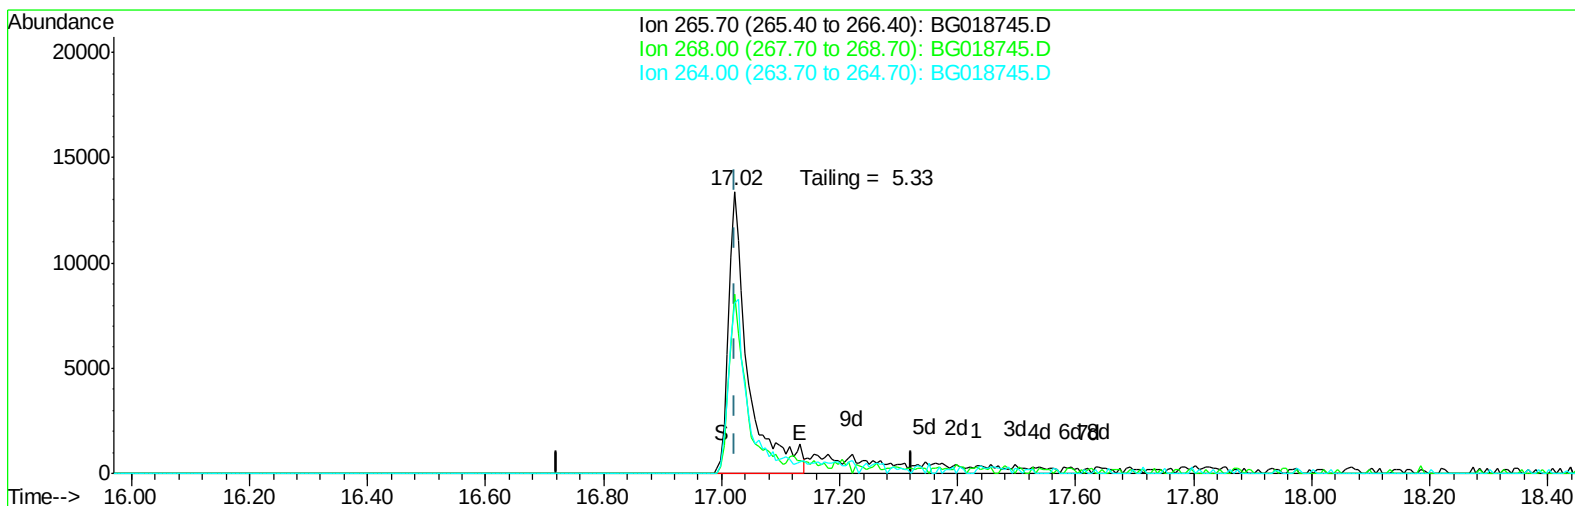

TIC: BG018745.D

(69) Pentachlorophenol (C)




17.433min (+0.411) 80.14ng

response 148

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	83.11#
264.00	60.10	44.59#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091815\
Data File : BG018745.D
Acq On : 17 Sep 2015 19:35
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 04:19:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 03:41:39 2015
Response via : Initial Calibration

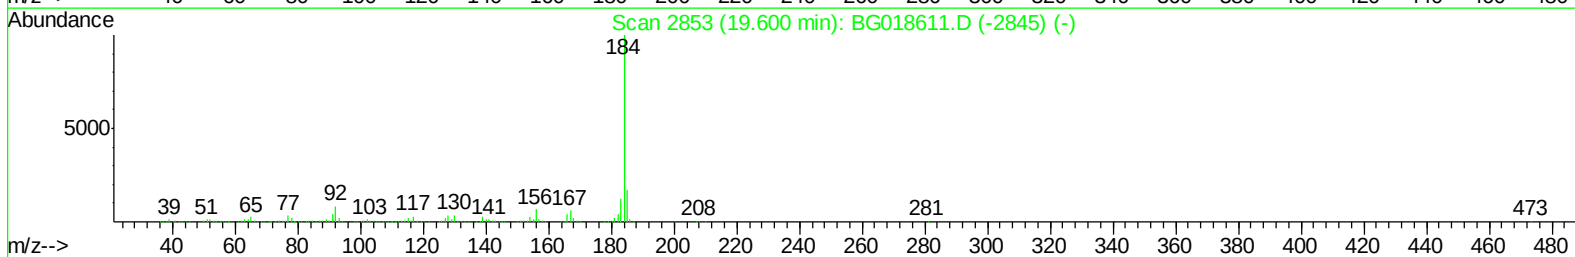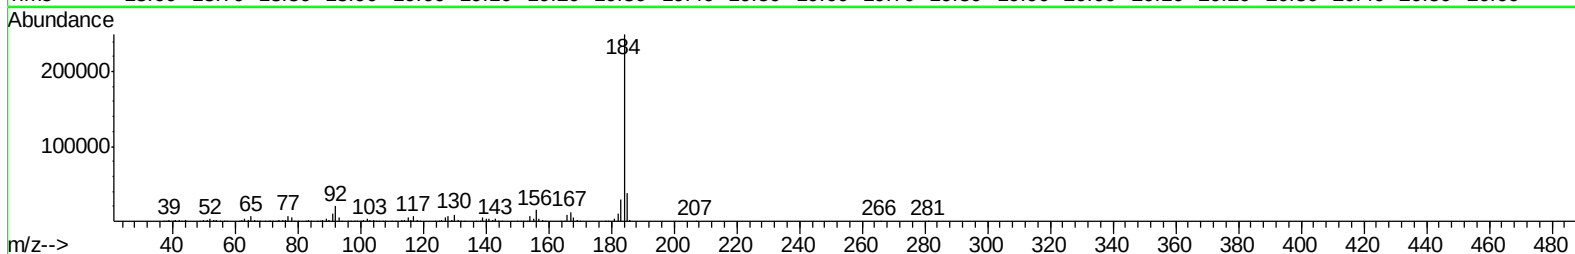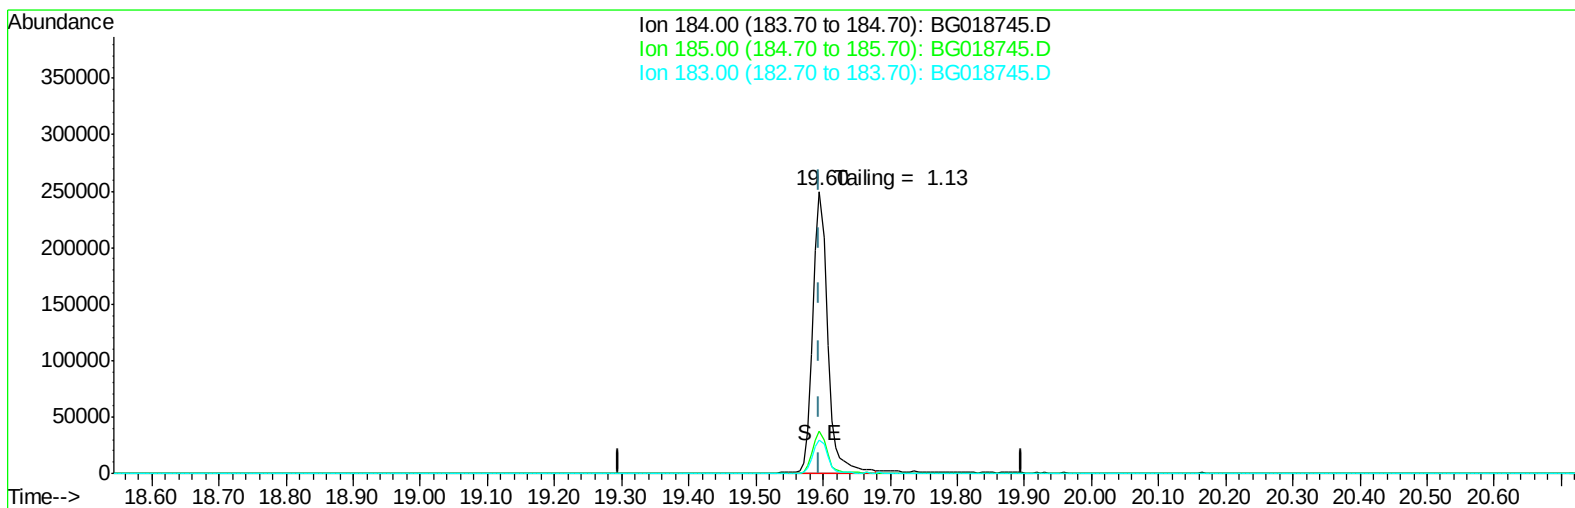

TIC: BG018745.D

(76) Benzidine

19.595min (-0.001) 0.00ng

response 369919

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.02
183.00	12.60	12.02
0.00	0.00	0.00