


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091815\
 Data File : BG018745.D
 Acq On : 17 Sep 2015 19:35
 Operator : TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 11 10:44:16 2015

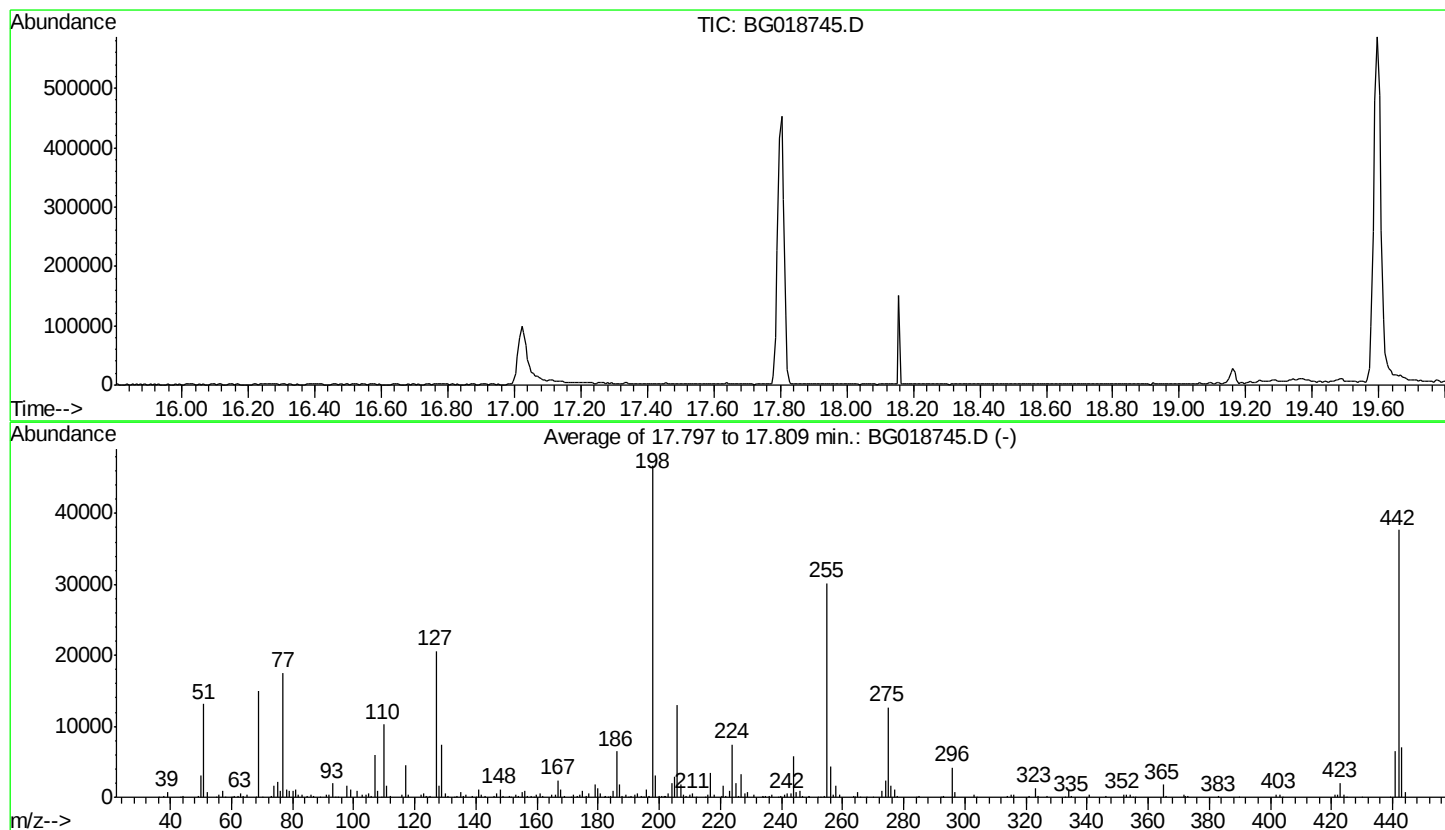

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	13155	PASS
68	69	0.00	2	0.6	92	PASS
69	198	0.00	100	32.0	14973	PASS
70	69	0.00	2	0.5	68	PASS
127	198	10	80	44.2	20645	PASS
197	198	0.00	2	0.2	77	PASS
198	198	100	100	100.0	46744	PASS
199	198	5	9	6.6	3073	PASS
275	198	10	60	27.1	12689	PASS
365	198	1	100	3.8	1767	PASS
441	442	0.01	24	17.1	6423	PASS
442	198	50	100	80.6	37653	PASS
443	442	15	24	18.8	7093	PASS