
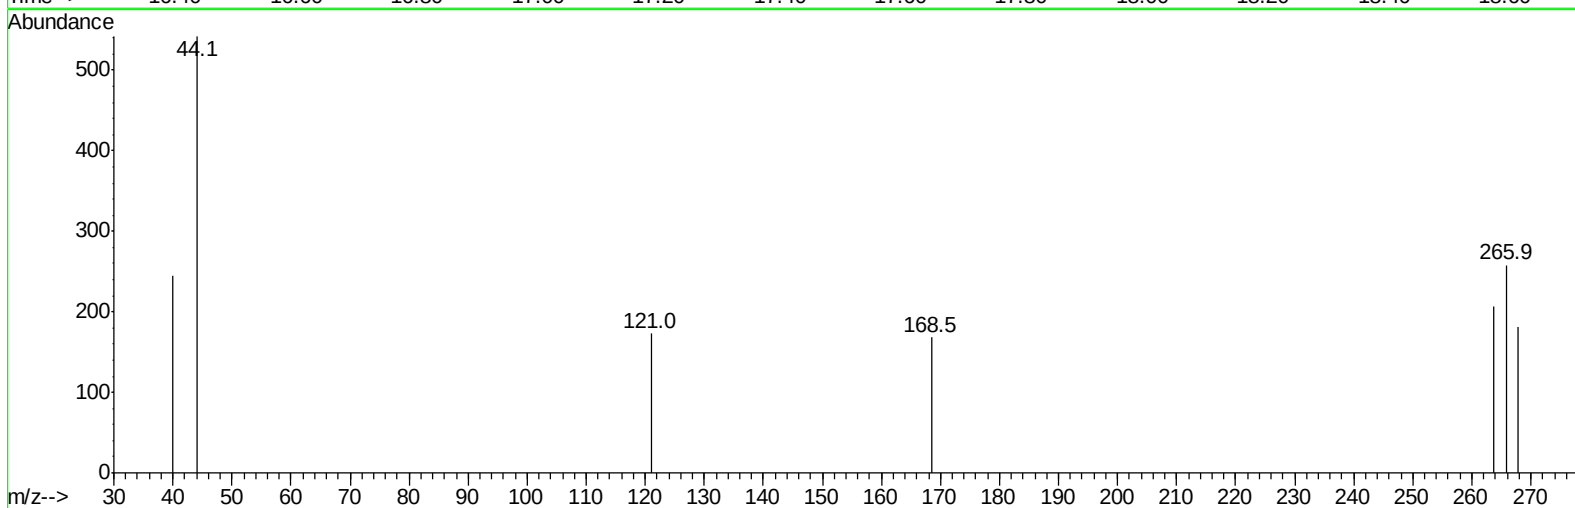


Data Path : Z:\HPCHEM1\BNA G\Data\BG091817\
Data File : BG028810.D
Acq On : 19 Sep 2017 00:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:27:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

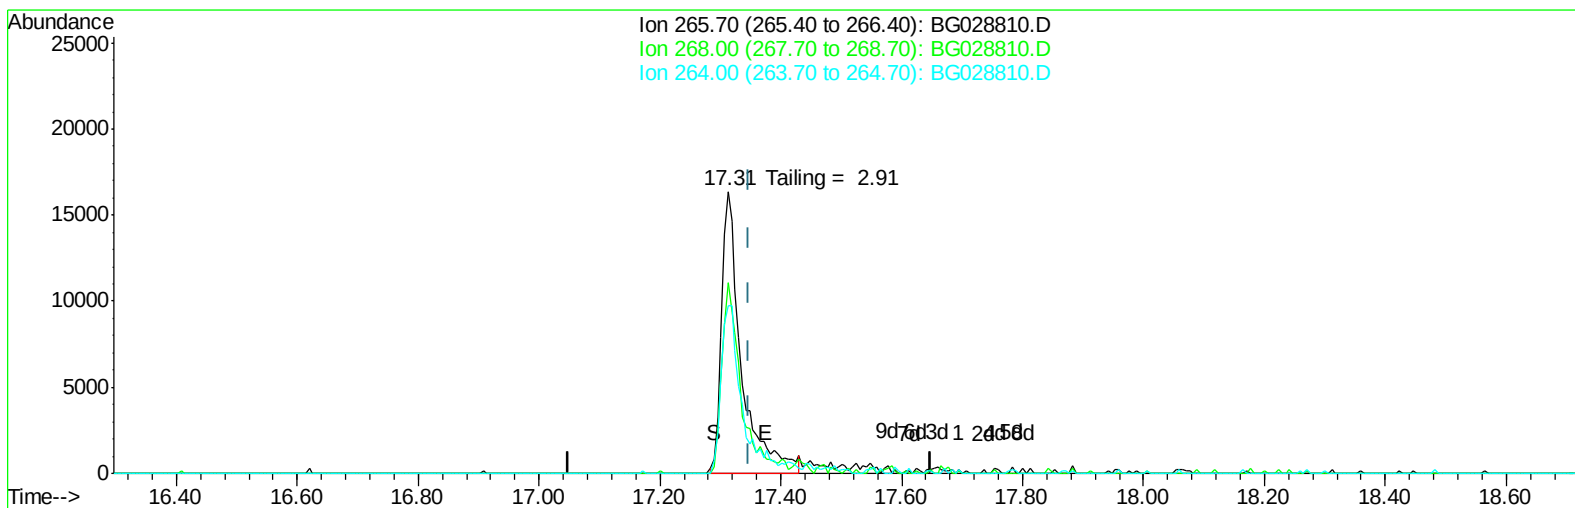

TIC: BG028810.D

(69) Pentachlorophenol (C)



17.695min (+0.346) 50.26ng

response 147

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	70.16
264.00	62.60	80.23#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG091817\
Data File : BG028810.D
Acq On : 19 Sep 2017 00:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:27:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

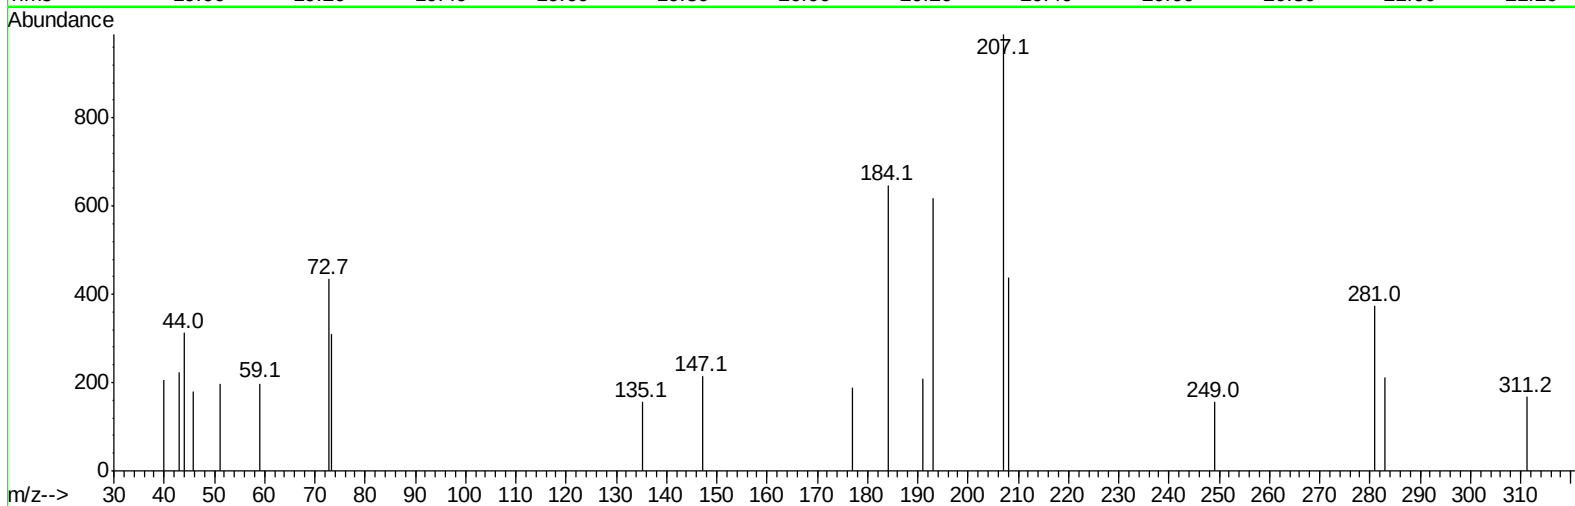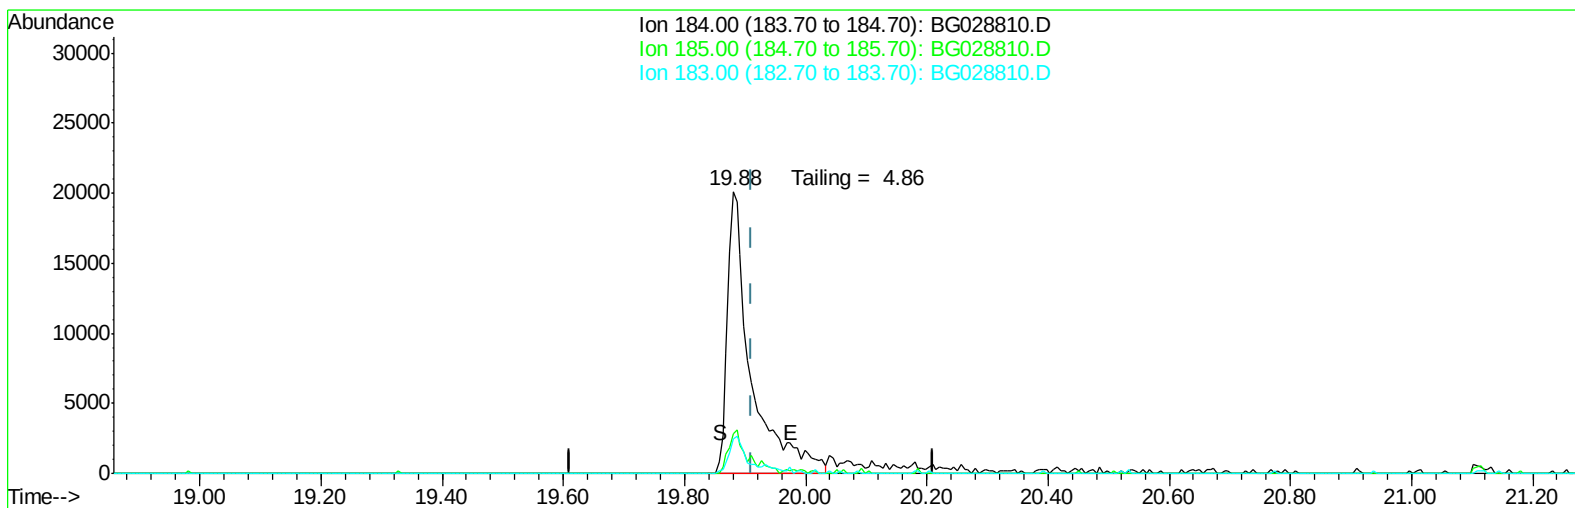

TIC: BG028810.D

(76) Benzidine

20.256min (+0.346) 286.46ng

response 624

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00