

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091817\
 Data File : BG028822.D
 Acq On : 19 Sep 2017 8:59
 Operator : SJ/JU
 Sample : I5265-20
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EQUIPMENT-BLANK-1

Quant Time: Sep 19 13:54:36 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	30591	20.00	ng	-0.04
21) Naphthalene-d8	11.11	136	122470	20.00	ng	-0.04
38) Acenaphthene-d10	14.91	164	92937	20.00	ng	-0.04
63) Phenanthrene-d10	17.66	188	258258	20.00	ng	-0.04
75) Chrysene-d12	21.98	240	284356	20.00	ng	-0.05
86) Perylene-d12	25.45	264	287951	20.00	ng	-0.08
System Monitoring Compounds						
5) 2-Fluorophenol	5.86	112	110982	59.86	ng	-0.05
7) Phenol-d6	7.44	99	95696	34.28	ng	-0.05
23) Nitrobenzene-d5	9.46	82	246007	96.09	ng	-0.05
41) 2,4,6-Tribromophenol	16.40	330	255591	166.28	ng	-0.04
44) 2-Fluorobiphenyl	13.53	172	670119	96.15	ng	-0.04
78) Terphenyl-d14	20.25	244	1265364	94.90	ng	-0.03


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091817\
Data File : BG028822.D
Acq On : 19 Sep 2017 8:59
Operator : SJ/JU
Sample : I5265-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EQUIPMENT-BLANK-1

Quant Time: Sep 19 13:54:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

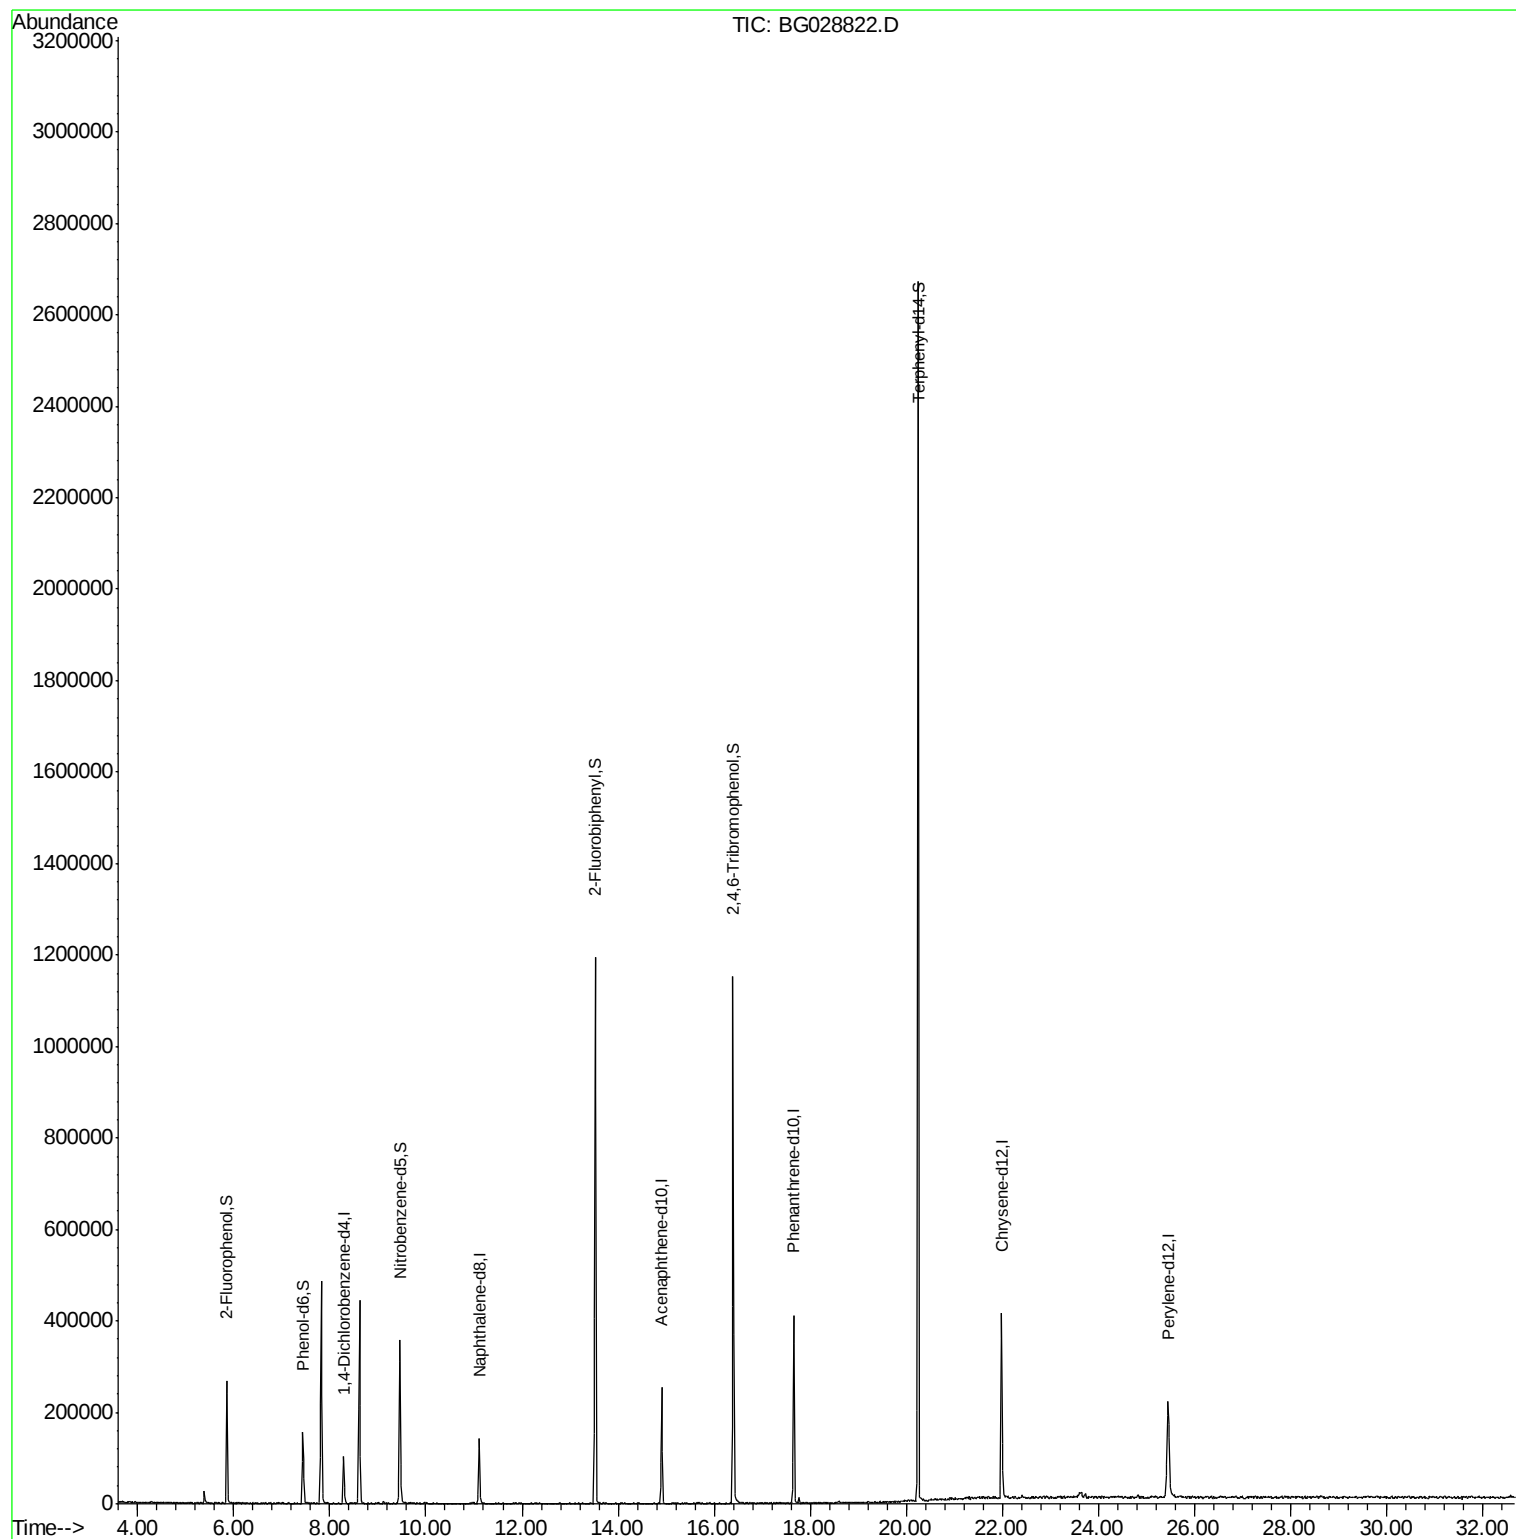



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.29 min Scan# 800

Delta R.T. -0.04 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Instrument :

BNA_G

ClientSampleId :

EQUIPMENT-BLANK-1


Tot Ion:152 Resp: 30591

Ion Ratio Lower Upper

152 100

150 142.0 114.0 171.0




115 62.5 48.1 72.1

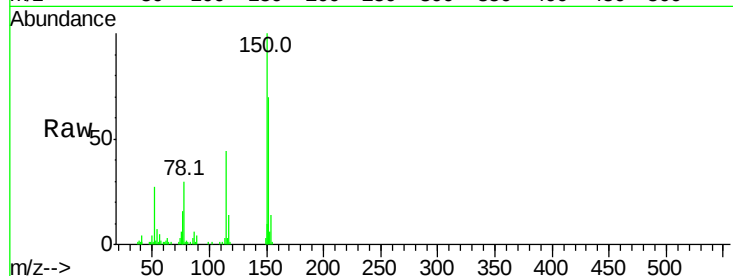

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

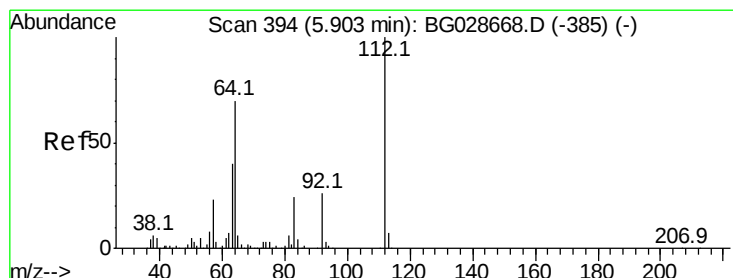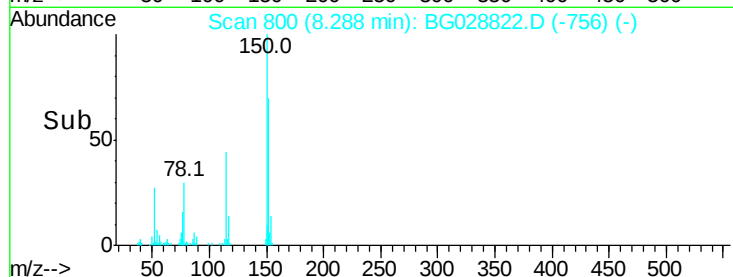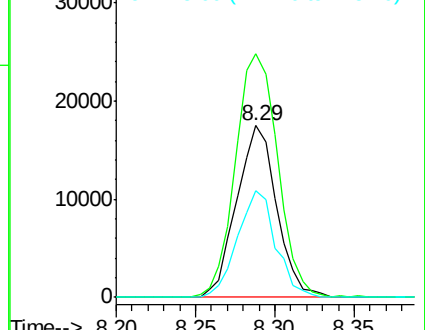

#5

2-Fluorophenol

Concen: 59.863 ng

RT: 5.86 min Scan# 386

Delta R.T. -0.05 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59


Tgt Ion:112 Resp: 110982

Ion Ratio Lower Upper

112 100

64 71.1 61.8 92.6



63 39.8 37.2 55.8

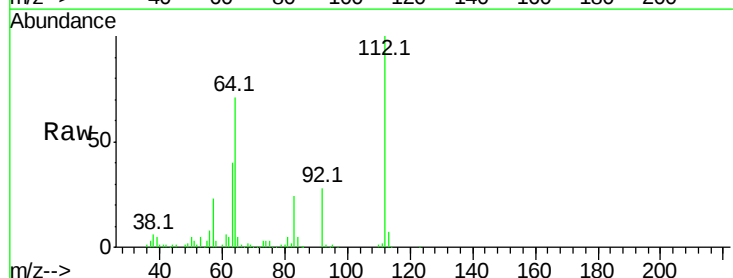

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

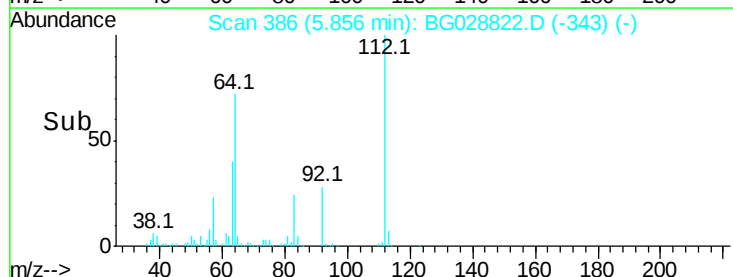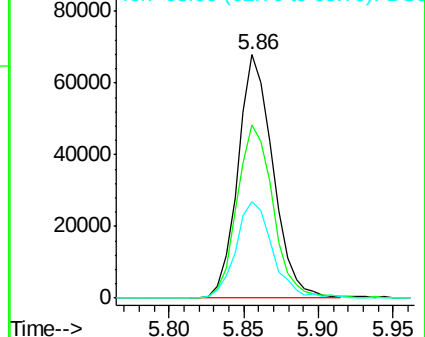



#7

Phenol-d6

Concen: 34.283 ng

RT: 7.44 min Scan# 656

Delta R.T. -0.05 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Instrument :

BNA_G

ClientSampleId :

EQUIPMENT-BLANK-1


Tot Ion: 99 Resp: 95696

Ion Ratio Lower Upper




99 100

42 19.1 20.5 30.7#

71 39.7 37.6 56.4

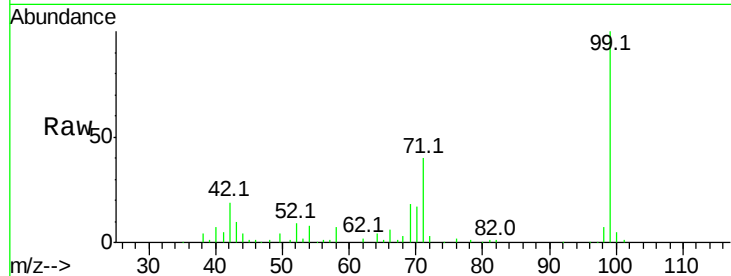

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

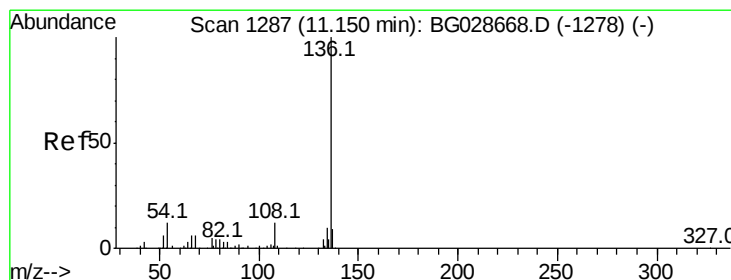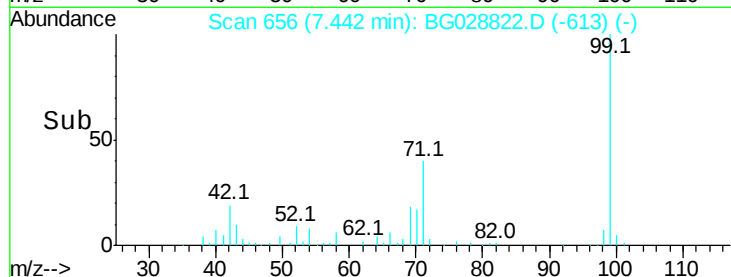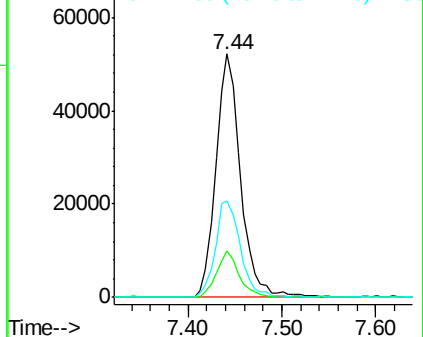

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.11 min Scan# 1280

Delta R.T. -0.04 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Tgt Ion: 136 Resp: 122470


Ion Ratio Lower Upper

136 100



137 12.4 8.9 13.3


54 11.0 9.3 13.9

68 5.4 5.1 7.7

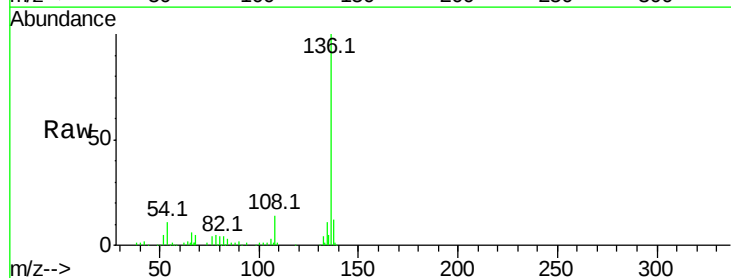

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

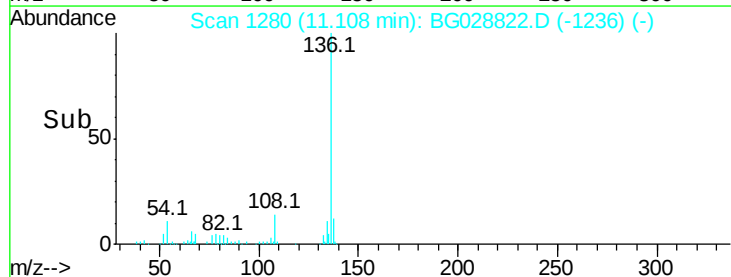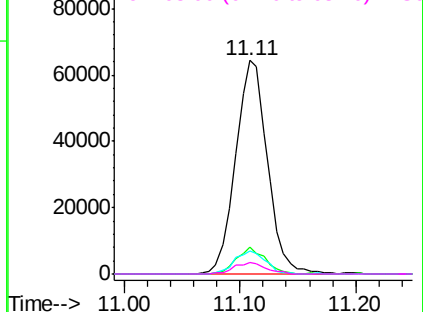

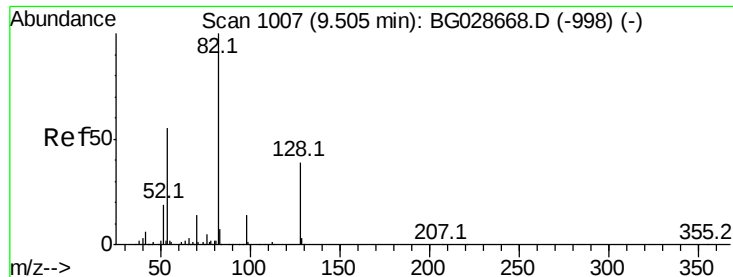

#23

Nitrobenzene-d5

Concen: 96.092 ng

RT: 9.46 min Scan# 999

Delta R.T. -0.05 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Instrument :

BNA_G

ClientSampleId :

EQUIPMENT-BLANK-1


Tot Ion: 82 Resp: 246007

Ion Ratio Lower Upper




82 100

128 37.6 26.4 39.6

54 56.0 49.4 74.2

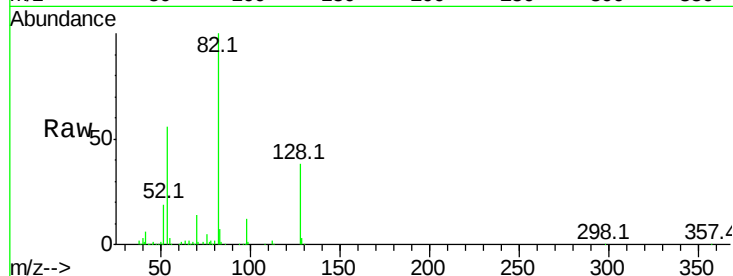

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

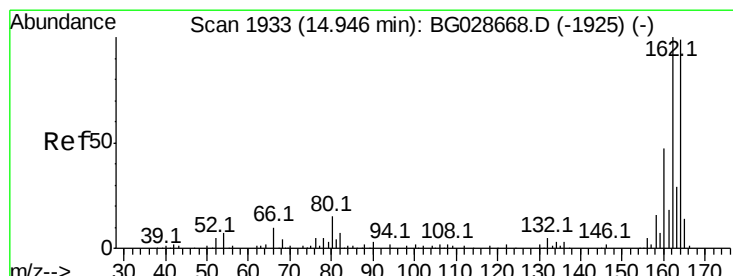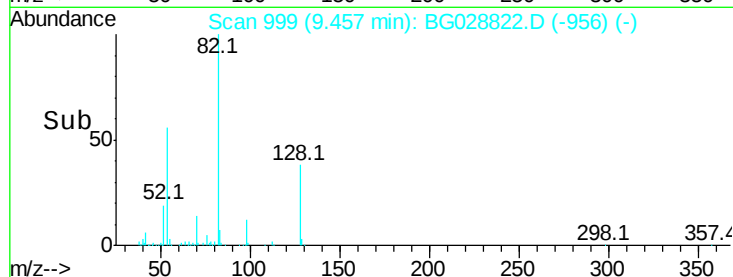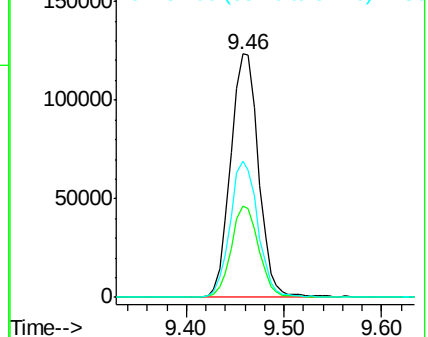

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.91 min Scan# 1927

Delta R.T. -0.04 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59


Tgt Ion: 164 Resp: 92937

Ion Ratio Lower Upper



164 100


162 102.5 85.1 127.7

160 46.7 34.7 52.1

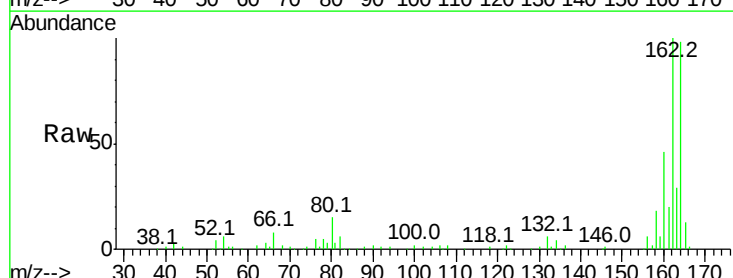

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

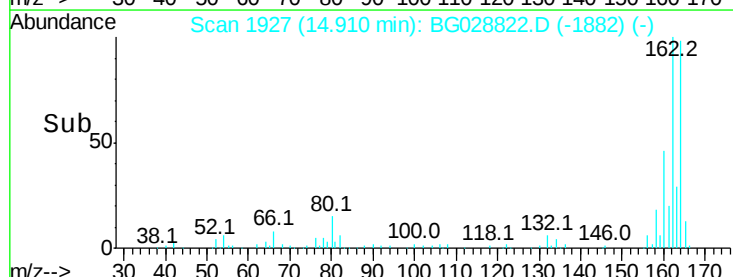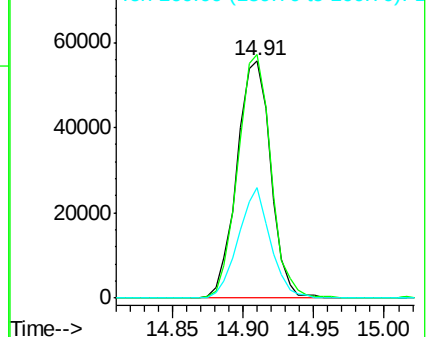


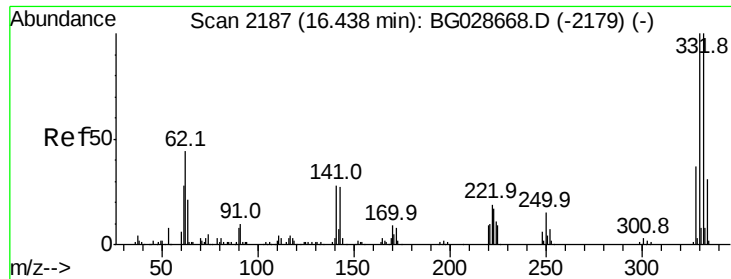




#41
 2,4,6-Tribromophenol
 Concen: 166.279 ng
 RT: 16.40 min Scan# 2181
 Delta R.T. -0.04 min
 Lab File: BG028822.D
 Acq: 19 Sep 2017 8:59

Instrument :
 BNA_G
 ClientSampleId :
 EQUIPMENT-BLANK-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	77.3	115.9
141	29.3	32.1	48.1#

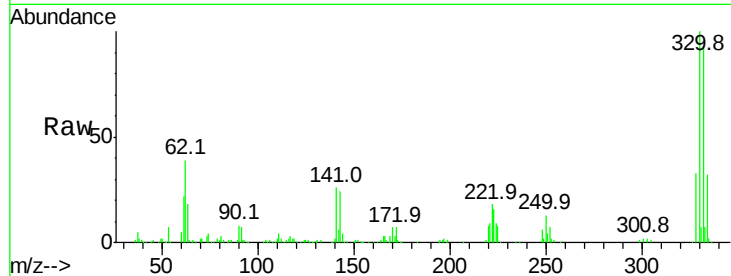


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

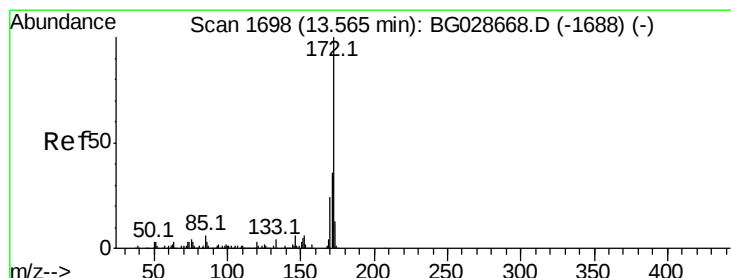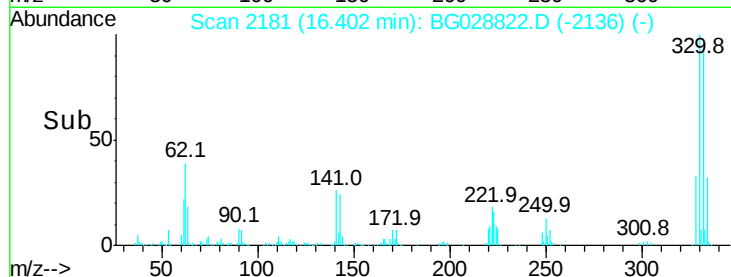
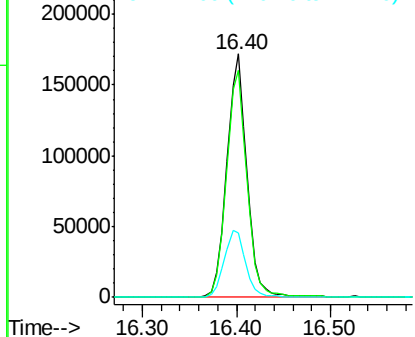


#44
 2-Fluorobiphenyl
 Concen: 96.146 ng
 RT: 13.53 min Scan# 1692
 Delta R.T. -0.04 min
 Lab File: BG028822.D
 Acq: 19 Sep 2017 8:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	32.2	48.2
170	21.8	21.8	32.6

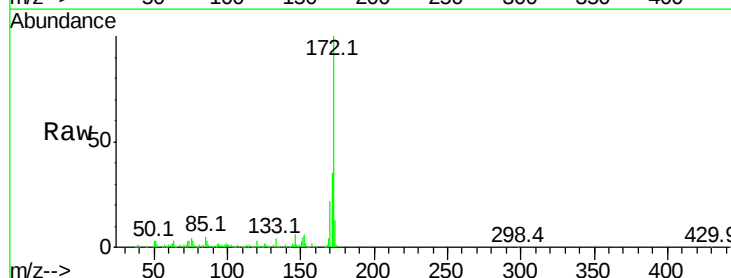

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

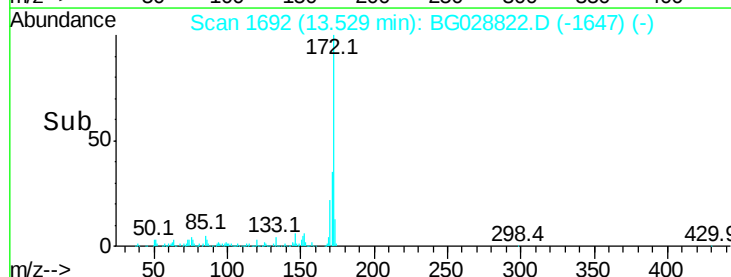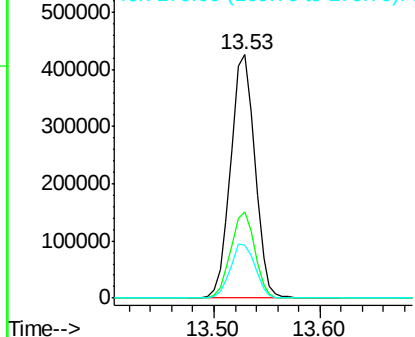



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.66 min Scan# 2395

Delta R.T. -0.04 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Instrument :

BNA_G

ClientSampleId :

EQUIPMENT-BLANK-1


Tot Ion:188 Resp: 258258

Ion Ratio Lower Upper

188 100

94 6.1 5.8 8.8



80 6.9 7.5 11.3#

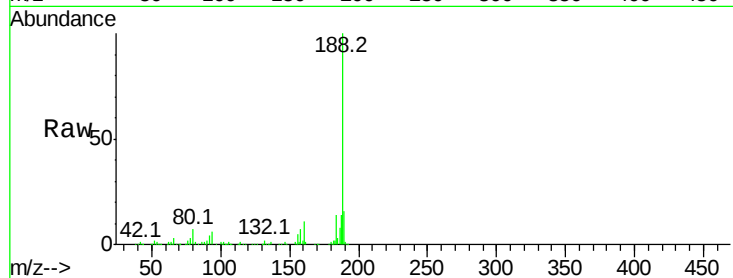

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

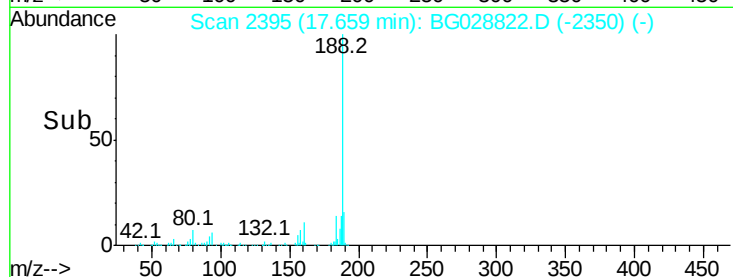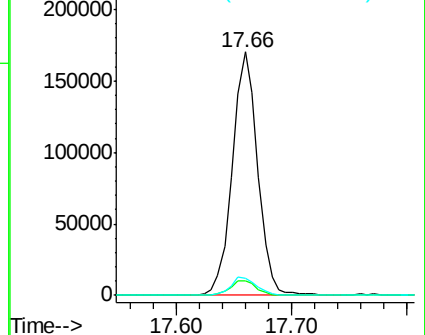

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.98 min Scan# 3131

Delta R.T. -0.05 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59


Tgt Ion:240 Resp: 284356

Ion Ratio Lower Upper

240 100

120 6.3 5.7 8.5



236 23.2 22.2 33.4

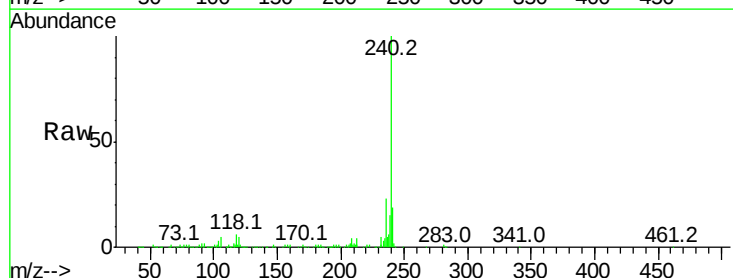


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

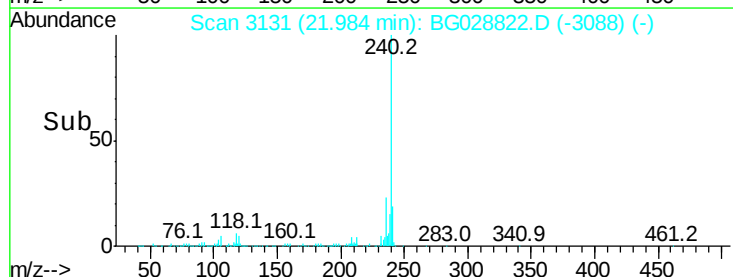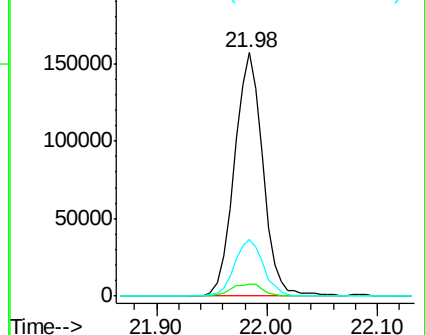

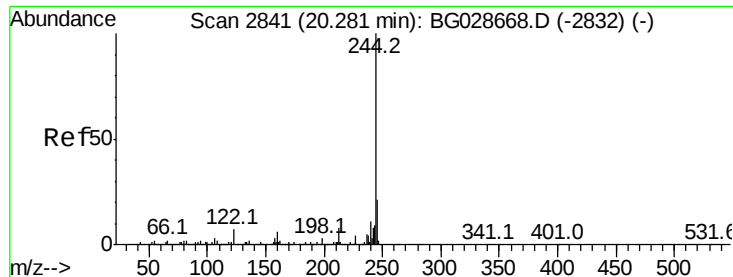

#78

Terphenyl-d14

Concen: 94.898 ng

RT: 20.25 min Scan# 2836

Delta R.T. -0.03 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Instrument :

BNA_G

ClientSampleId :

EQUIPMENT-BLANK-1





Tot Ion:244 Resp: 1265364

Ion Ratio Lower Upper

244 100

212 7.8 10.0 15.0#

122 6.9 8.6 12.8#

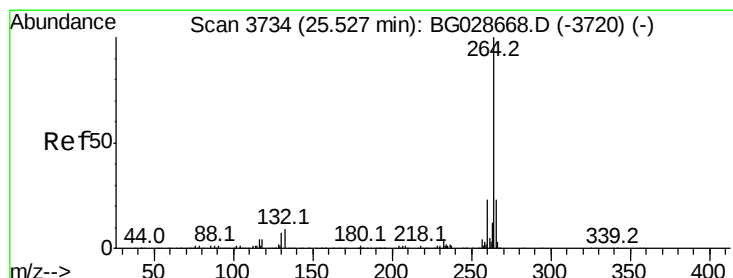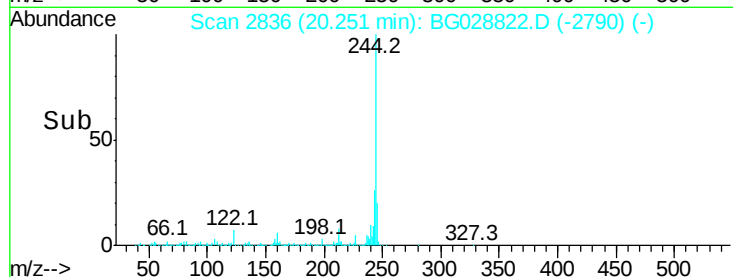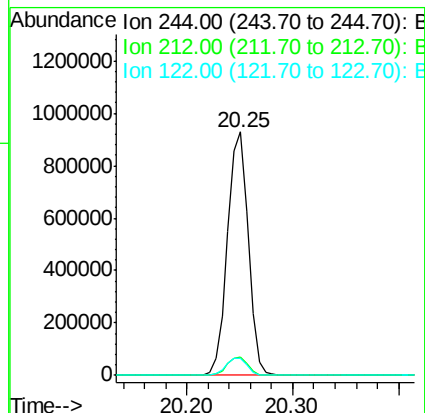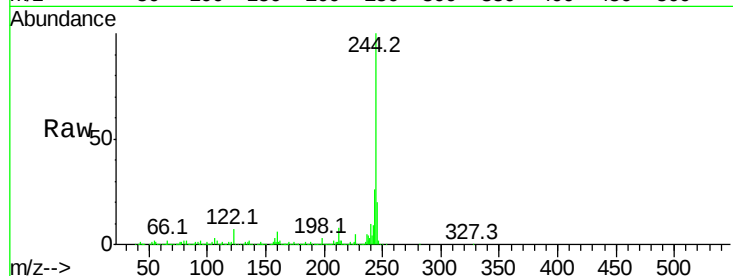

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.45 min Scan# 3721

Delta R.T. -0.08 min

Lab File: BG028822.D

Acq: 19 Sep 2017 8:59

Tgt Ion:264 Resp: 287951

Ion Ratio Lower Upper

264 100

260 24.4 21.8 32.8

265 20.7 18.2 27.4

