
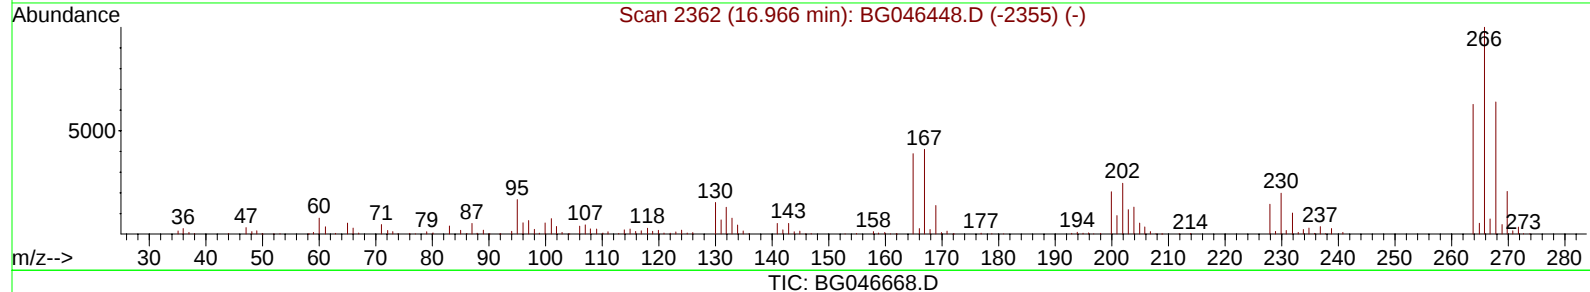
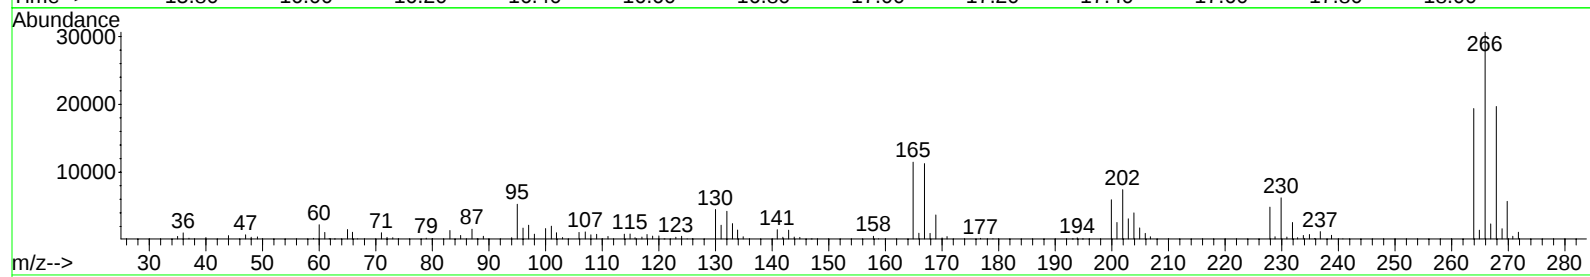


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091820\
Data File : BG046668.D
Acq On : 18 Sep 2020 12:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 13:33:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 17 14:27:03 2020
Response via : Initial Calibration

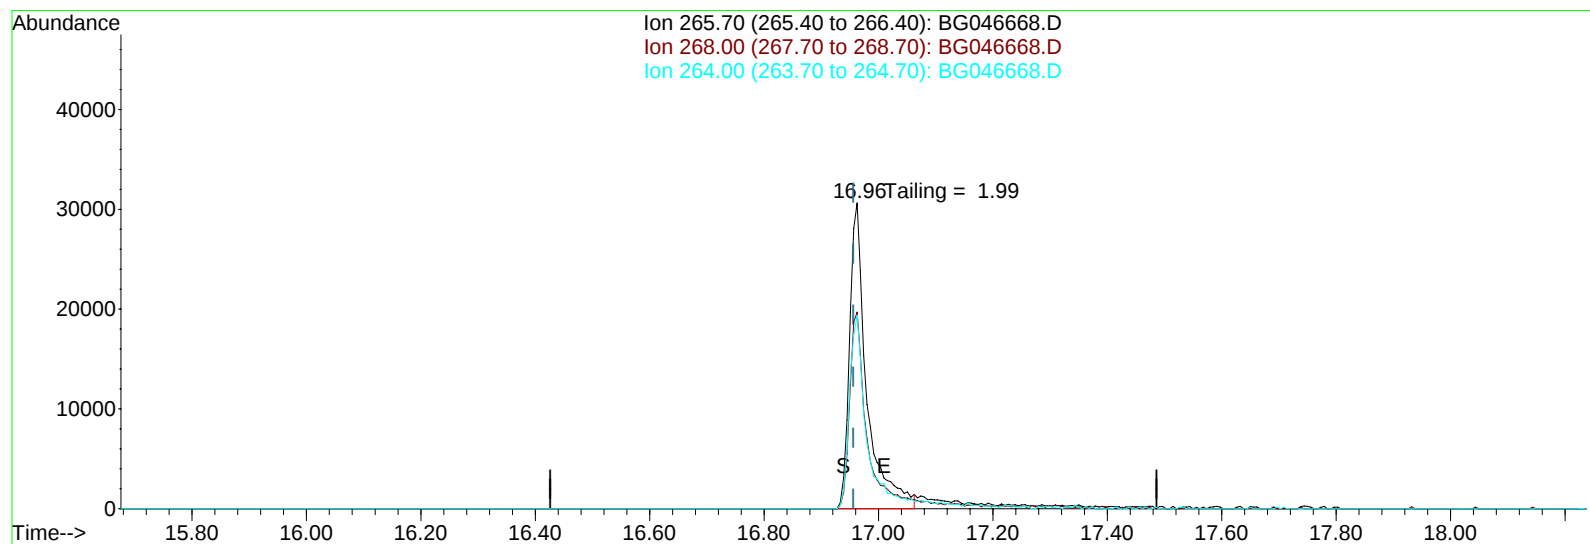

(70) Pentachlorophenol (C)




16.962min (+0.007) 30287.15ng

response 68495

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.30
264.00	61.60	63.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091820\
Data File : BG046668.D
Acq On : 18 Sep 2020 12:03
Operator : CG/JU
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 13:33:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 17 14:27:03 2020
Response via : Initial Calibration

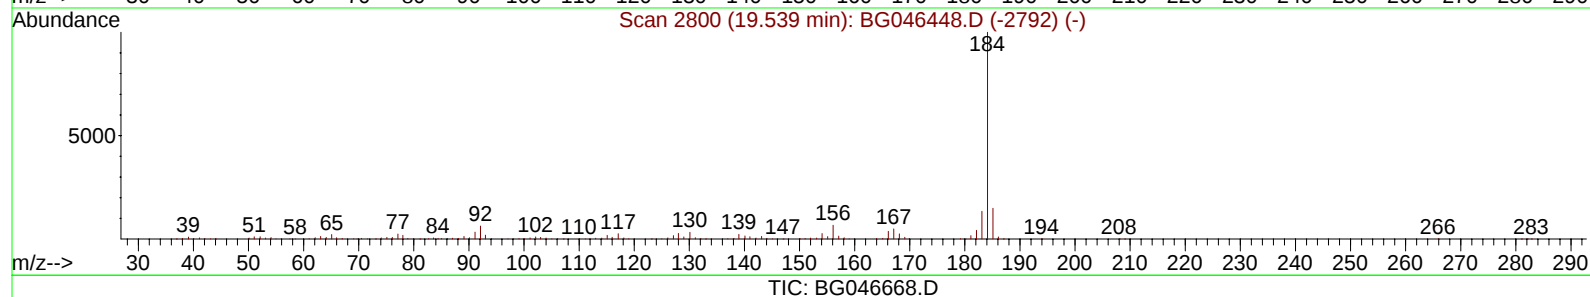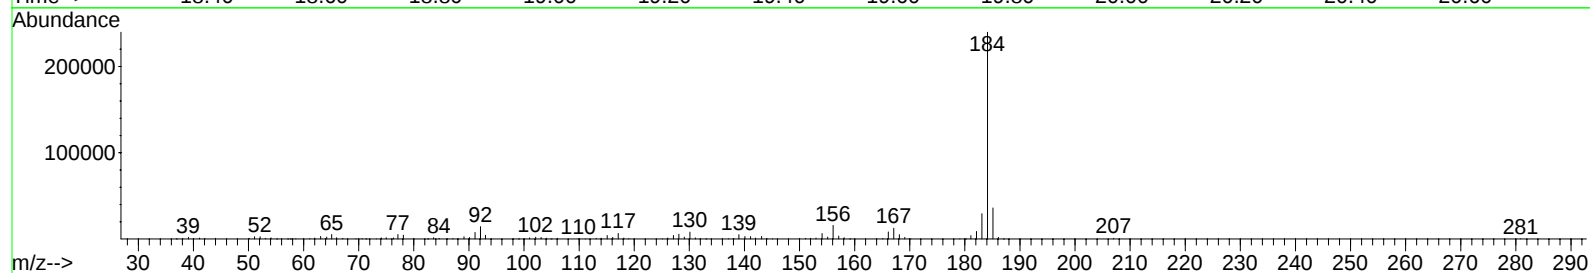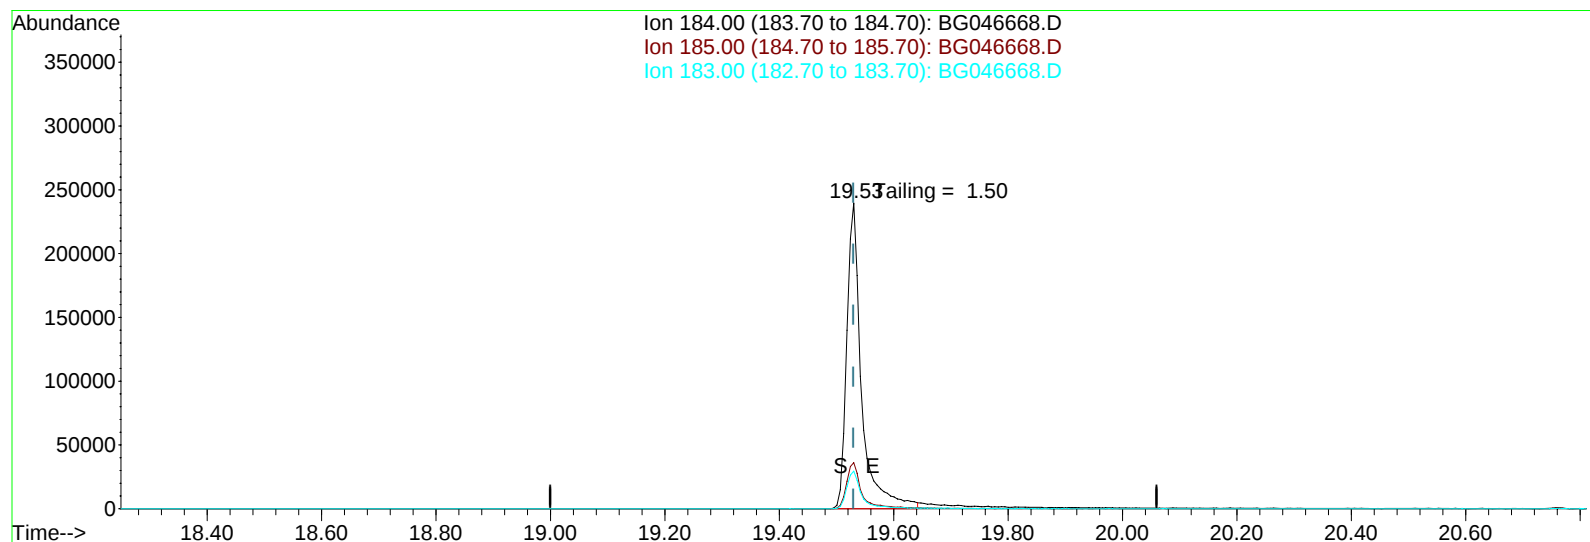

(77) Benzidine

19.530min (+0.001) 0.00ng

response 445234

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.05
183.00	13.20	12.29
0.00	0.00	0.00