


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091820\
 Data File : BG046668.D
 Acq On : 18 Sep 2020 12:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 17 14:27:03 2020

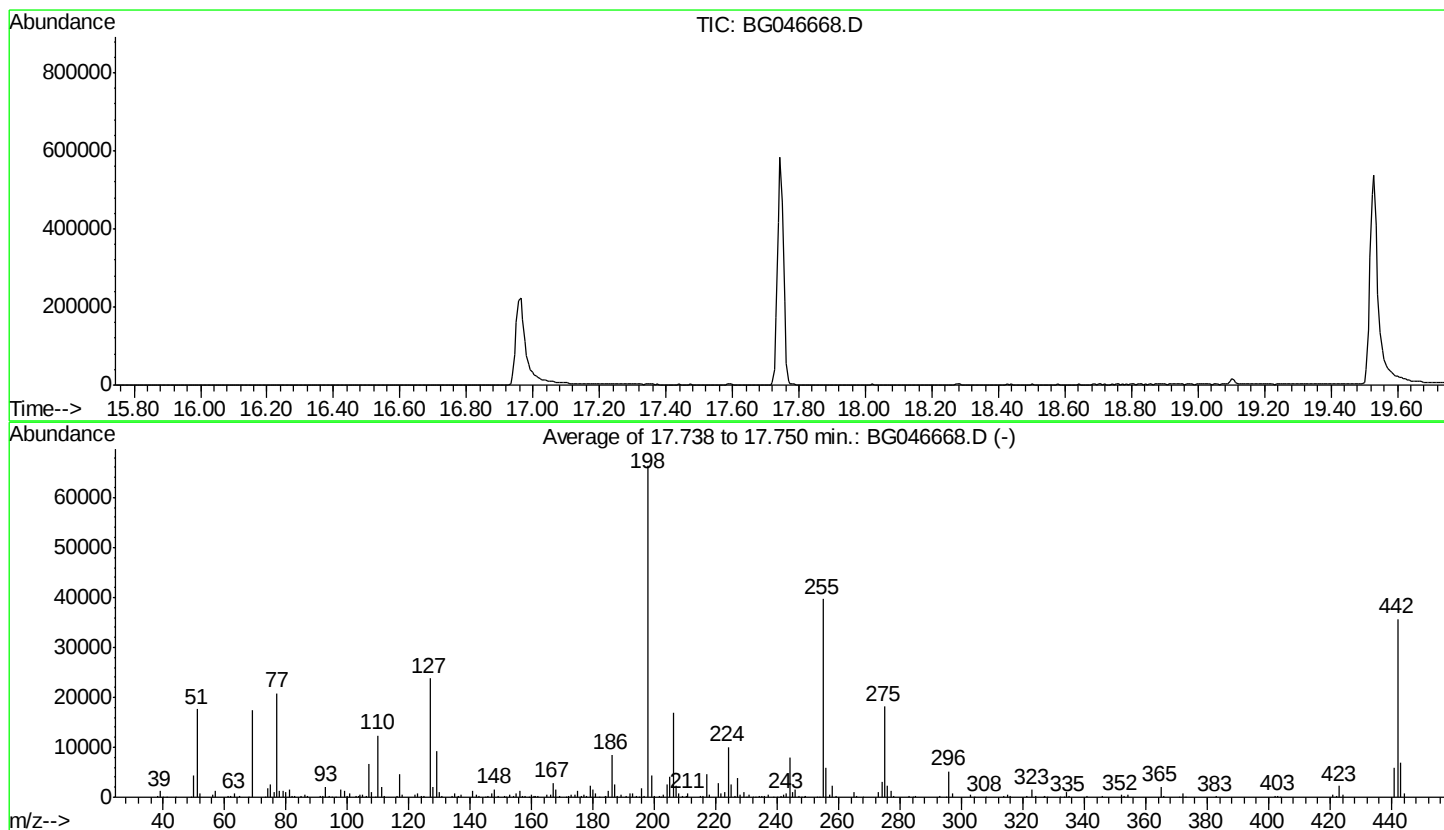

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	17637	PASS
68	69	0.00	2	0.6	101	PASS
69	198	0.00	100	26.2	17409	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.9	23818	PASS
197	198	0.00	2	0.2	143	PASS
198	198	100	100	100.0	66378	PASS
199	198	5	9	6.5	4323	PASS
275	198	10	60	27.3	18114	PASS
365	198	1	100	3.3	2171	PASS
441	198	0.01	100	9.0	5986	PASS
442	198	50	100	53.8	35722	PASS
443	442	15	24	19.3	6912	PASS