
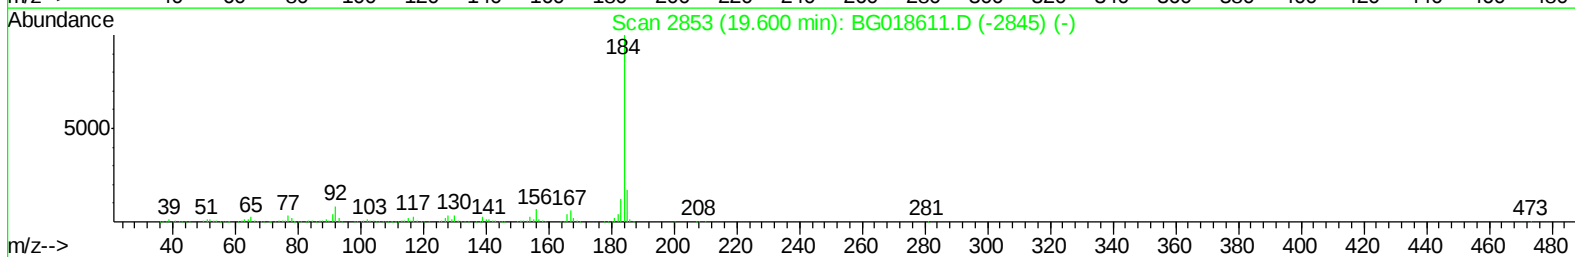
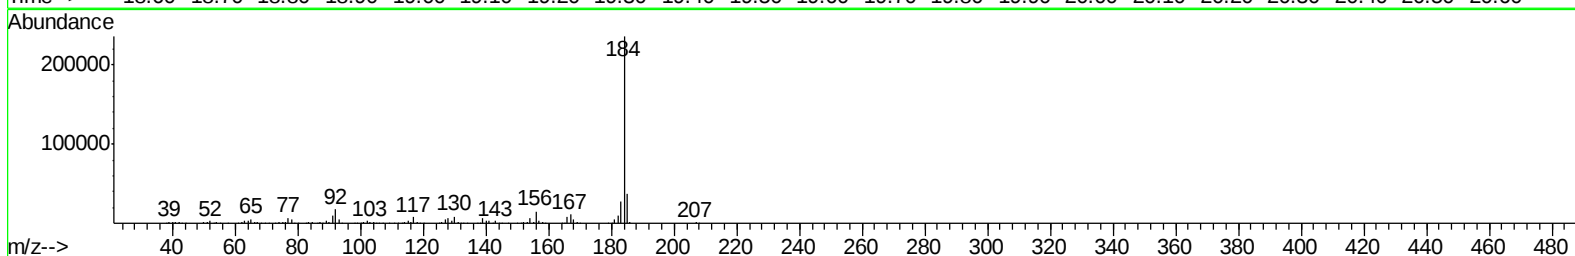


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091915\
Data File : BG018759.D
Acq On : 18 Sep 2015 8:39
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Sep 19 01:40:41 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 23:51:57 2015
Response via : Initial Calibration

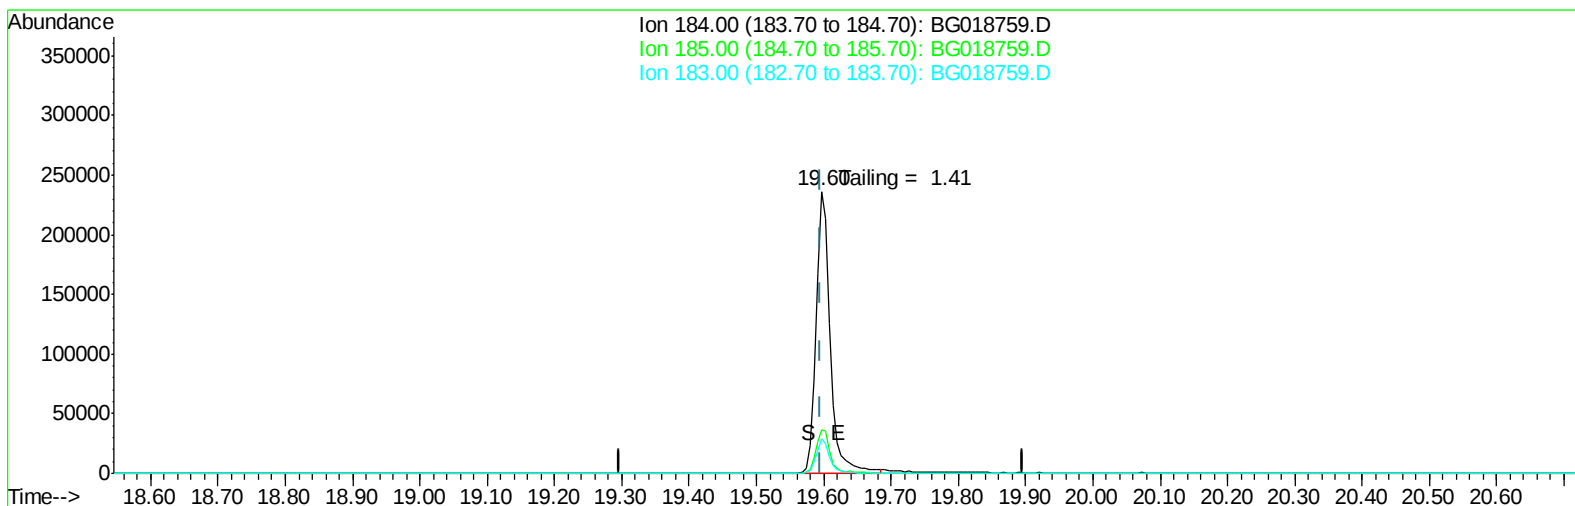

TIC: BG018759.D

(76) Benzidine

19.597min (-0.000) 77482.58ng




response 358328

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.55
183.00	12.60	12.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG091915\
Data File : BG018759.D
Acq On : 18 Sep 2015 8:39
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Sep 19 01:40:41 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 23:51:57 2015
Response via : Initial Calibration

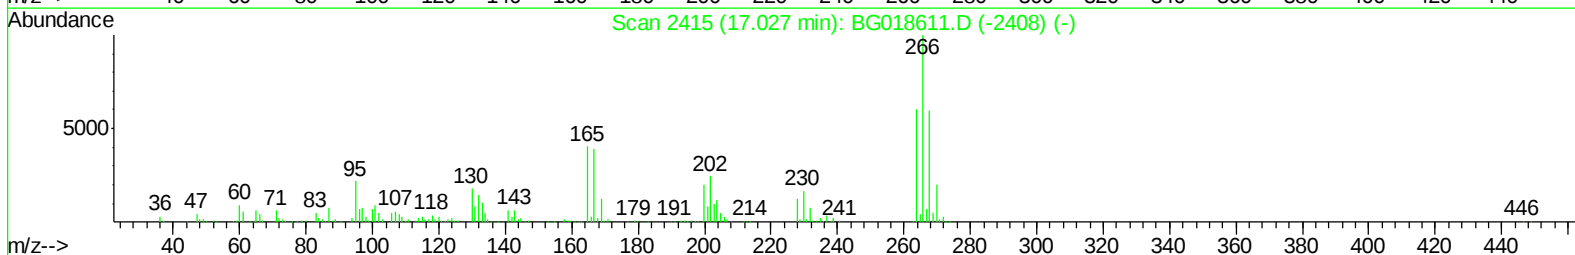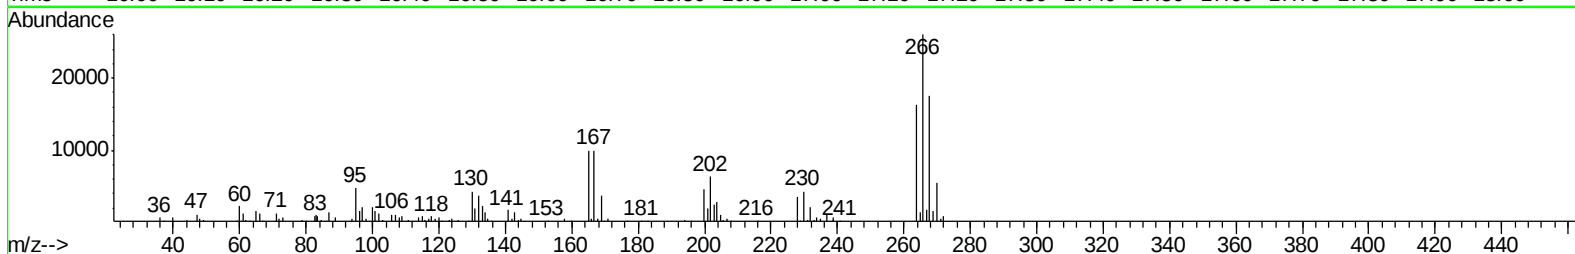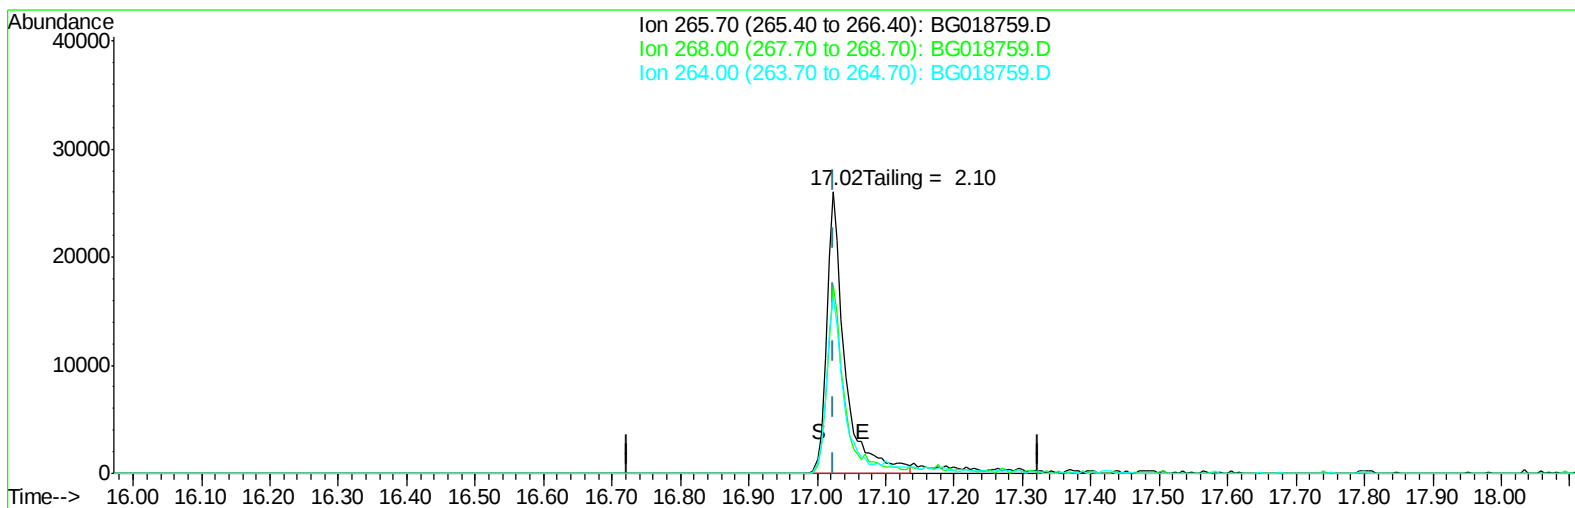

TIC: BG018759.D

(69) Pentachlorophenol (C)

17.023min (-0.000) 96046.45ng

response 47126

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	67.06
264.00	60.10	62.71
0.00	0.00	0.00