


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091915\
Data File : BG018759.D
Acq On : 18 Sep 2015 8:39
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 11 10:44:16 2015

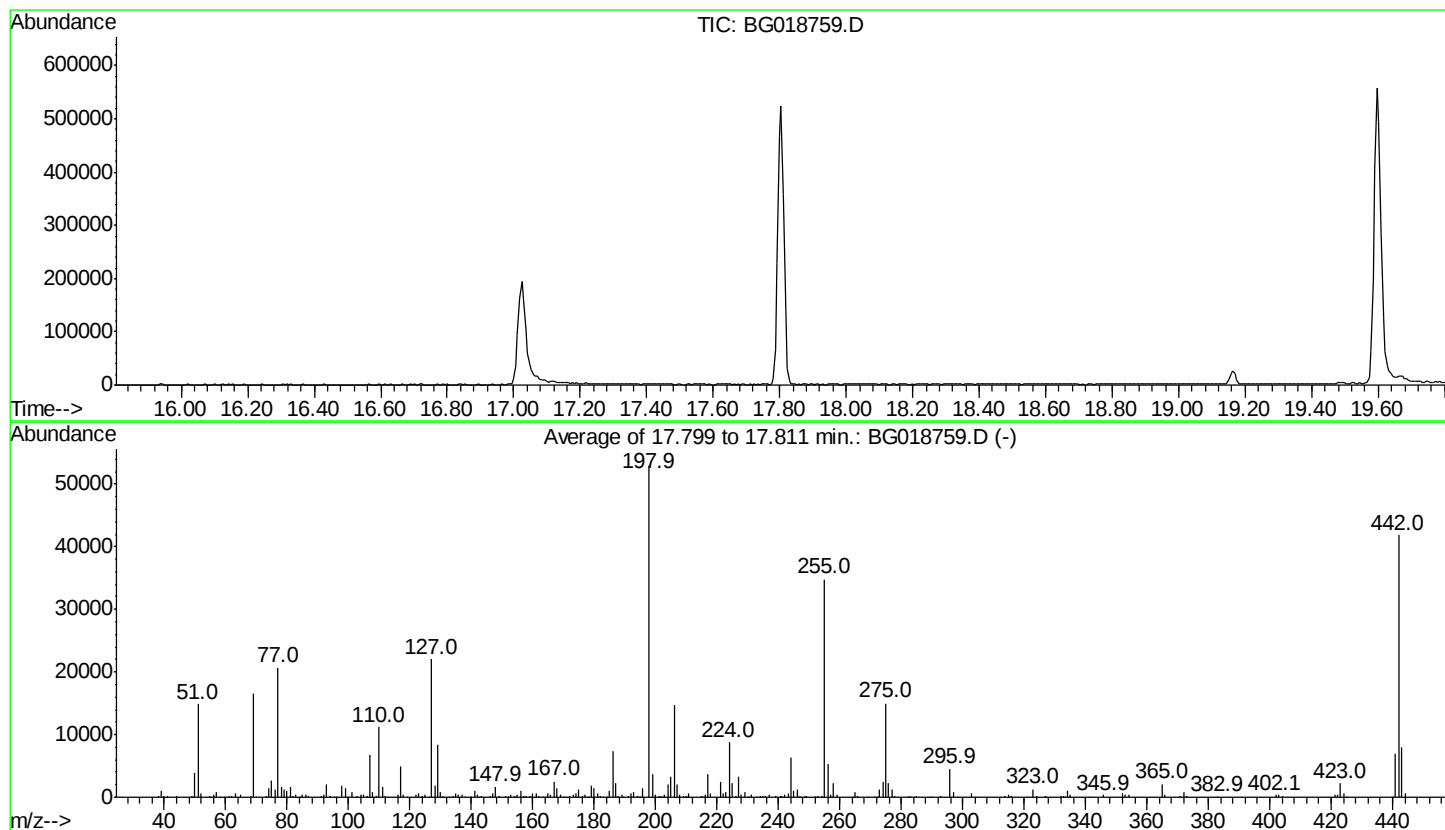

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	14889	PASS
68	69	0.00	2	1.7	282	PASS
69	198	0.00	100	31.2	16500	PASS
70	69	0.00	2	0.4	66	PASS
127	198	10	80	41.6	22007	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52949	PASS
199	198	5	9	7.1	3737	PASS
275	198	10	60	28.4	15021	PASS
365	198	1	100	3.9	2073	PASS
441	442	0.01	24	16.7	7007	PASS
442	198	50	100	79.1	41874	PASS
443	442	15	24	19.3	8078	PASS